

Minimizing noise during fMRI acquisition

Daniel Handwerker

June 25, 2018



NOISE !?

- “Impacting the effect of fMRI **noise** through hardware and acquisition choices – Implications for controlling false positive rates”
Wald & Polimeni, *NeuroImage* (2017)
- First sentence of their introduction
 - Applied to the intensity fluctuations of a pixel in an fMRI time-series, the term “noise” is so non-specific and carries such negative connotations that it should probably be eliminated from the fMRI vocabulary.


What causes noise?

- Measurement errors
 - Thermal Noise (MRI physics)
 - “Under sampled” data
- Imperfect data processing
 - Assumptions in data recon algorithms – particularly with acceleration
- Imperfect signal modeling
 - Not acquiring or mis-using undesired fluctuations
 - Bad alignment between images



What do we mean by minimizing noise?

- Maximize Signal-To-Noise Ratio (SNR)
- Maximize Temporal Signal-To-Noise Ratio (TSNR)
- Maximize Contrast-To-Noise Ratio (CNR)



High SNR

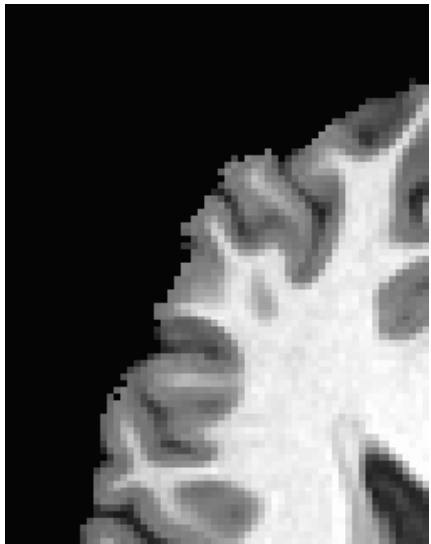

Low SNR

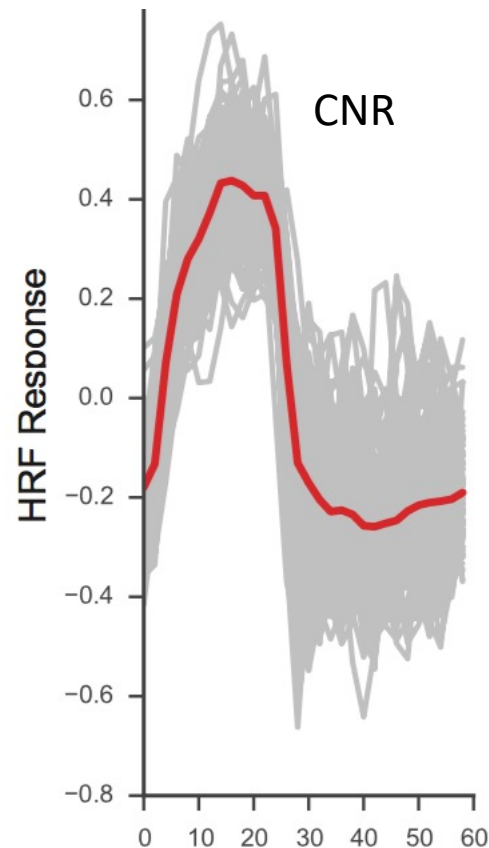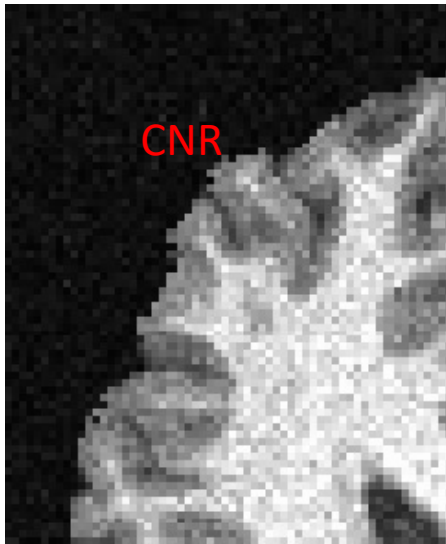


TSNR

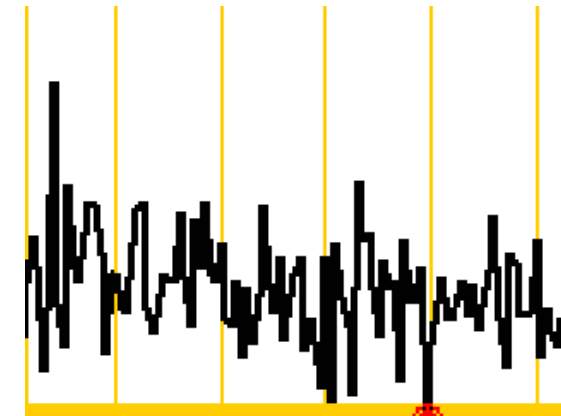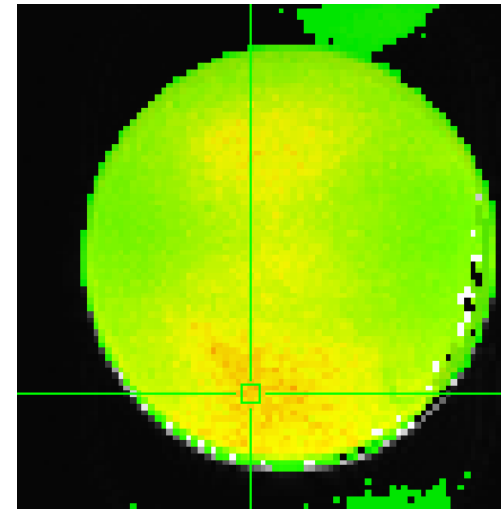

What do we mean by minimizing noise?

- Minimize specific artifacts
- Minimize distortions & signal dropout

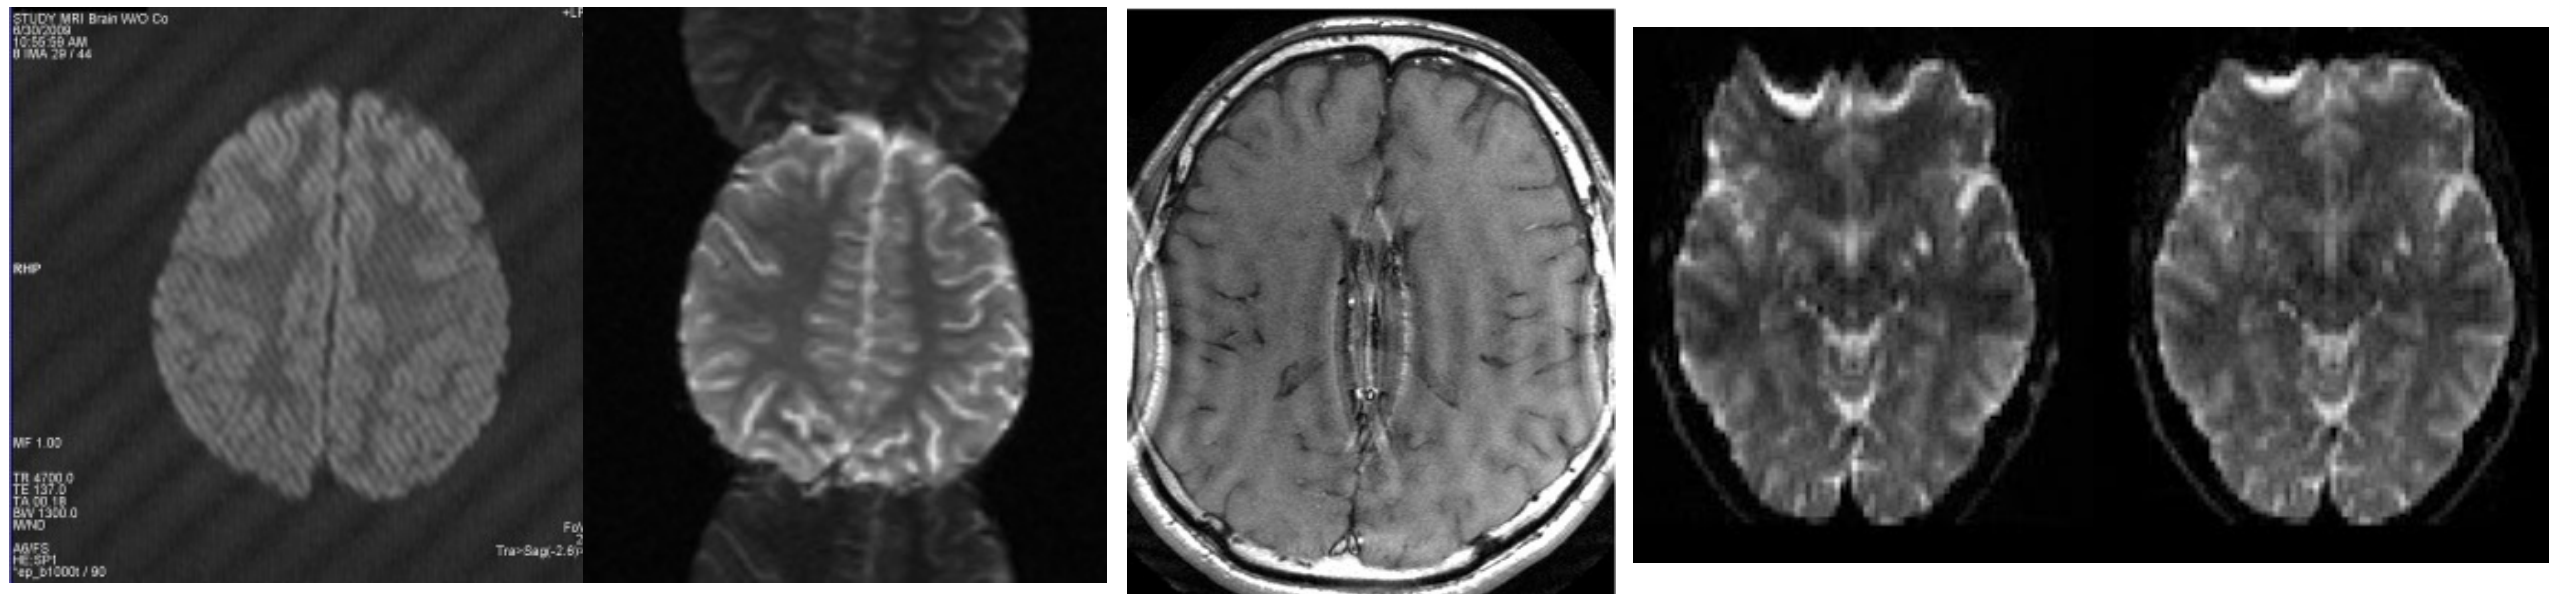

<http://www.24x7mag.com/2014/01/abcs-mri/>
<http://mriquestions.com/nyquist-n2-ghosts.html>
<http://mriquestions.com/artifacts-in-pi.html>
<https://practicalfmri.blogspot.com/2011/11/physics-for-understanding-fmri.html>



What do we mean by minimizing noise?

Minimize subject-induced or unmodeled variation

- Head movement
- Breathing, Heart pulsation, chest movement
- Unmodeled behavior or neural activity
 - task non-compliance
 - Non-task specific structured behaviors
- Unmodeled Hemodynamic Responses / Neurovascular Coupling

What do we mean by minimizing noise?

- Improve temporal resolution
- Improve spatial specificity

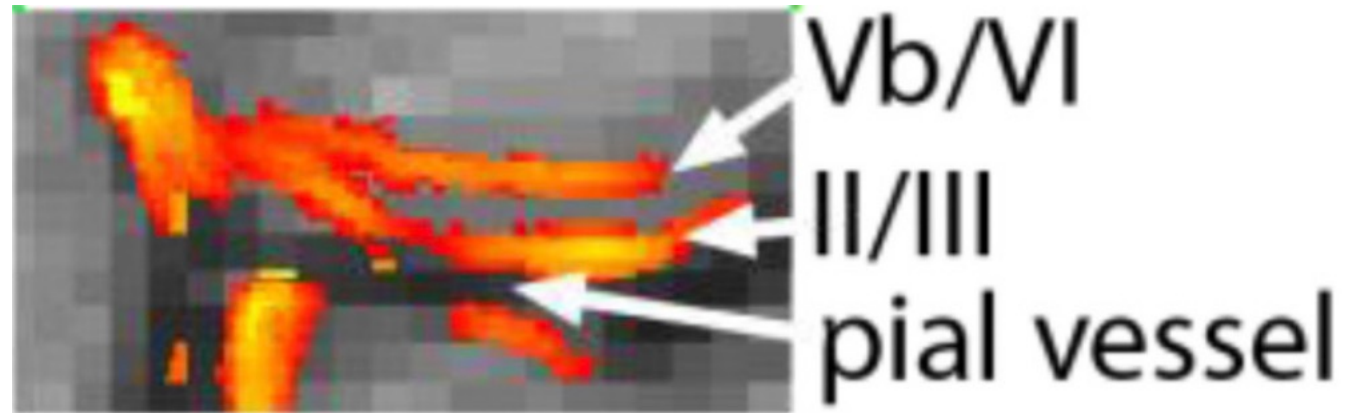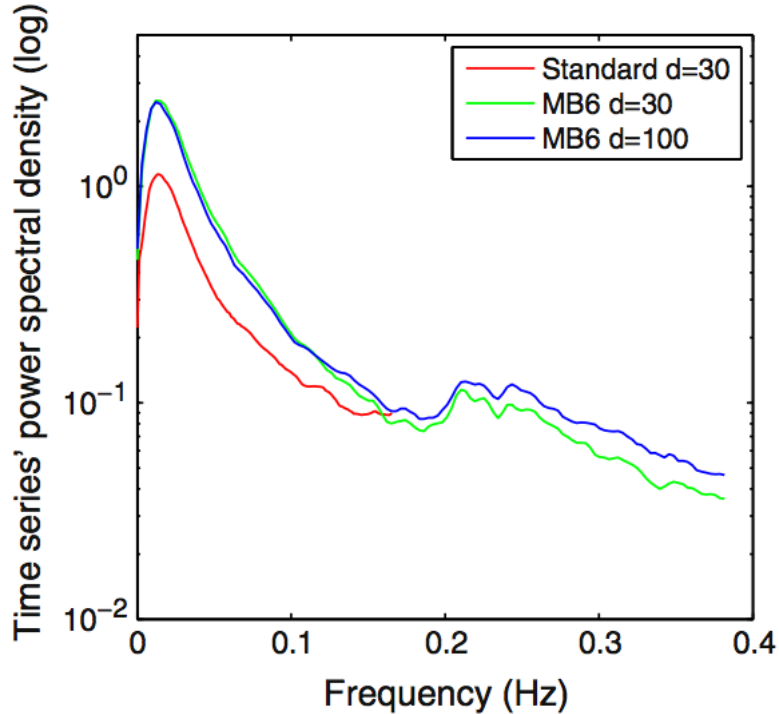

Huber et al NeuroImage (in press)

What do we mean by minimizing noise?

- Maximize Signal-To-Noise Ratio (SNR)
- Maximize Contrast-To-Noise Ratio (CNR)
- Maximize Temporal Signal-To-Noise Ratio (TSNR)
- Minimize specific artifacts
- Minimize distortions & signal dropout
- Minimize subject-induced or unmodeled variation
- Improve temporal resolution
- Improve spatial specificity

We want fast data at super high resolution where responses can be resolved in just a few trials with no distortion, dropout, or artifacts

Everything is a balance of priorities with no definitive right answer, but many wrong ones

Parts of Presentation

- Parameters & Pulse Sequences
- Peripherals & Participants
- Preventative scanner health

Parameters and Pulse Sequences



A semi-arbitrary and semi-ordered series of examples

- Examples of how parameter choices matter
- Preparatory scans matter
- SMS vs 3D-EPI
- Contrast options
- Motion correction
- Calibration scans

General acquisition goals

- Give thought to the specific priorities of a study
 - Response shape sensitivity vs specificity
 - Anatomical accuracy
 - Robustness against general artifacts
 - Robustness against artifacts that can bias a study
- The optimal acquisition options aren't always obvious.
 - What is the best flip angle for an fMRI study?


Optimal flip angle?

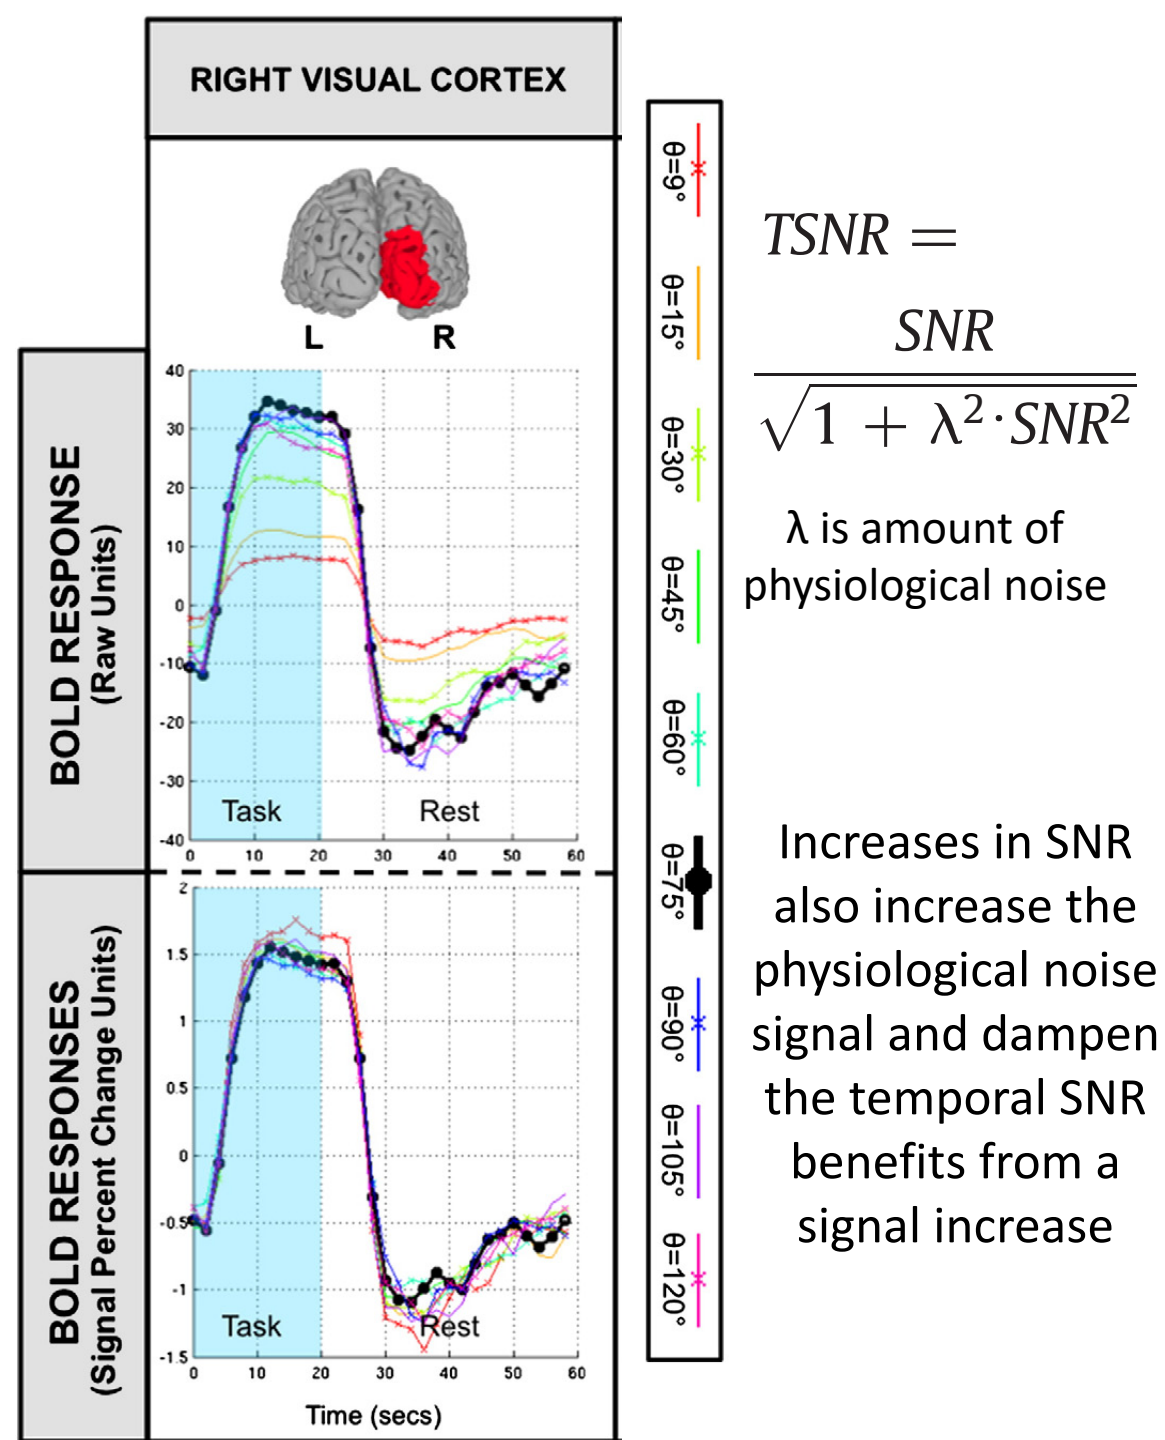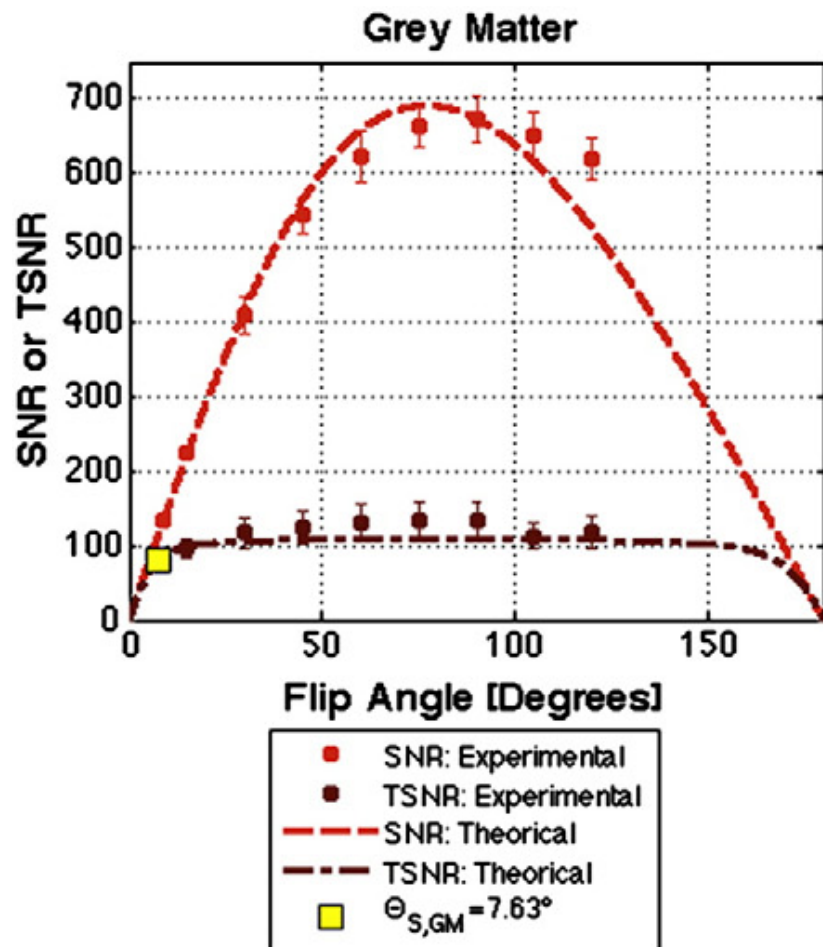

MRI acquisition general parameters

- Voxel size
 - Smaller -> Lower SNR
 - Smaller -> More anatomical specificity -> Higher TSNR of interest


$3 \times 3 \times 3 \text{ mm}^3$ voxels = 27 mm^3
 $1 \times 1 \times 1 \text{ mm}^3$ voxels = 1 mm^3

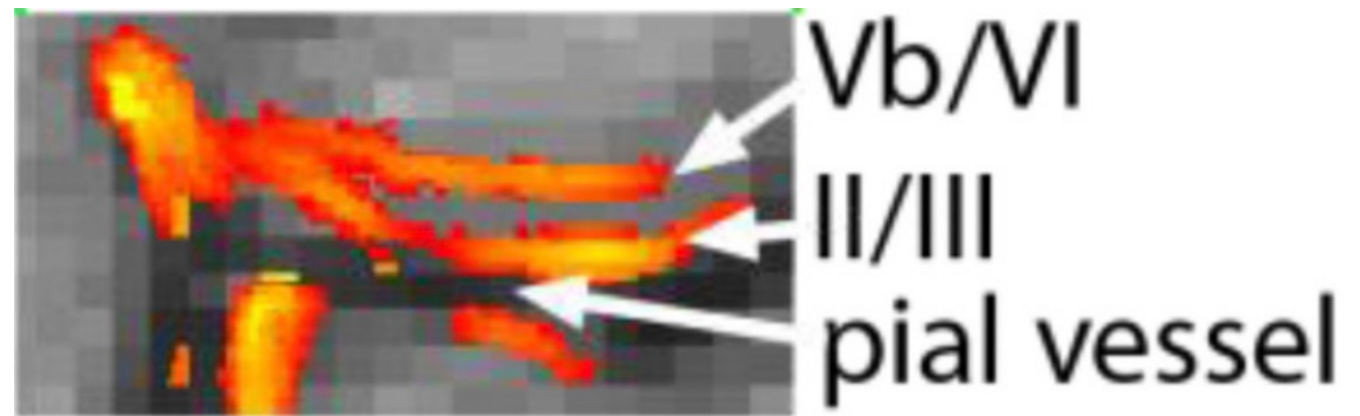


Huber et al NeuroImage (in press)

MRI acquisition general parameters

- TR
 - Shorter -> lower SNR, but better temporal resolution and possibly higher TSNR
 - Shorter -> Better filtering of high frequency artifacts (if not removed using other methods)
 - Still limited by the speed of the hemodynamic response

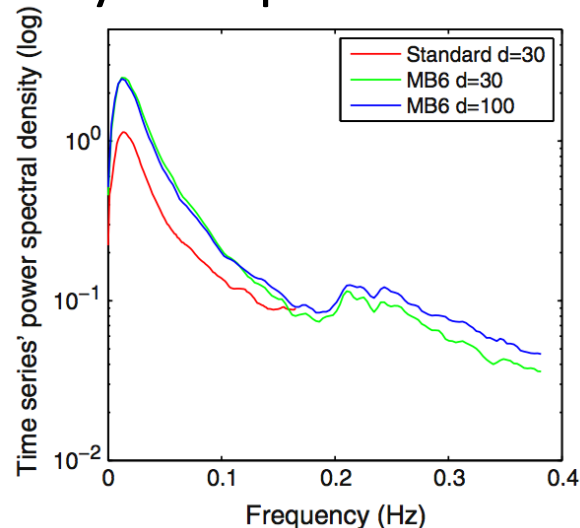

Griffanti et al NeuroImage 2014

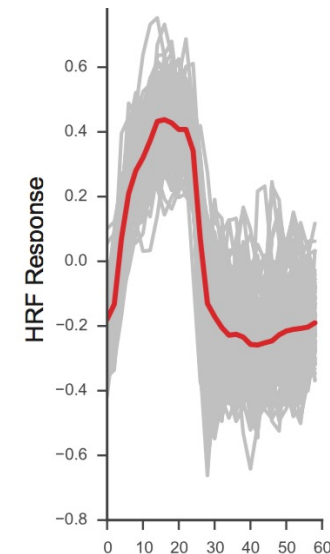


MRI acquisition general parameters



- Acceleration (collecting incompletely sampled data sets and estimating what was missing during reconstruction)
 - Sometimes lower SNR
 - Makes shorter TRs, smaller voxels, and multi-echo practical
 - Potentially less susceptibility dropout & distortion
 - Imperfect reconstruction can create or amplify artifacts
 - Possibly more sensitivity to B0 fluctuations linked to respiratory chest movement

GRAPPA acceleration reconstruction affected by calibration scan

Conventional EPI calibration scan
can contain phase errors

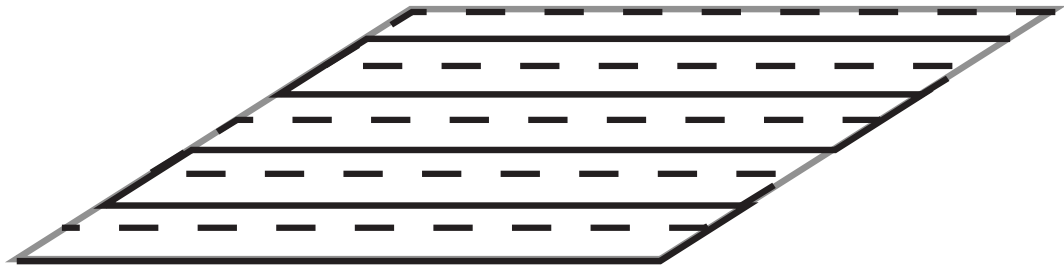


FLASH calibration scan is more robust

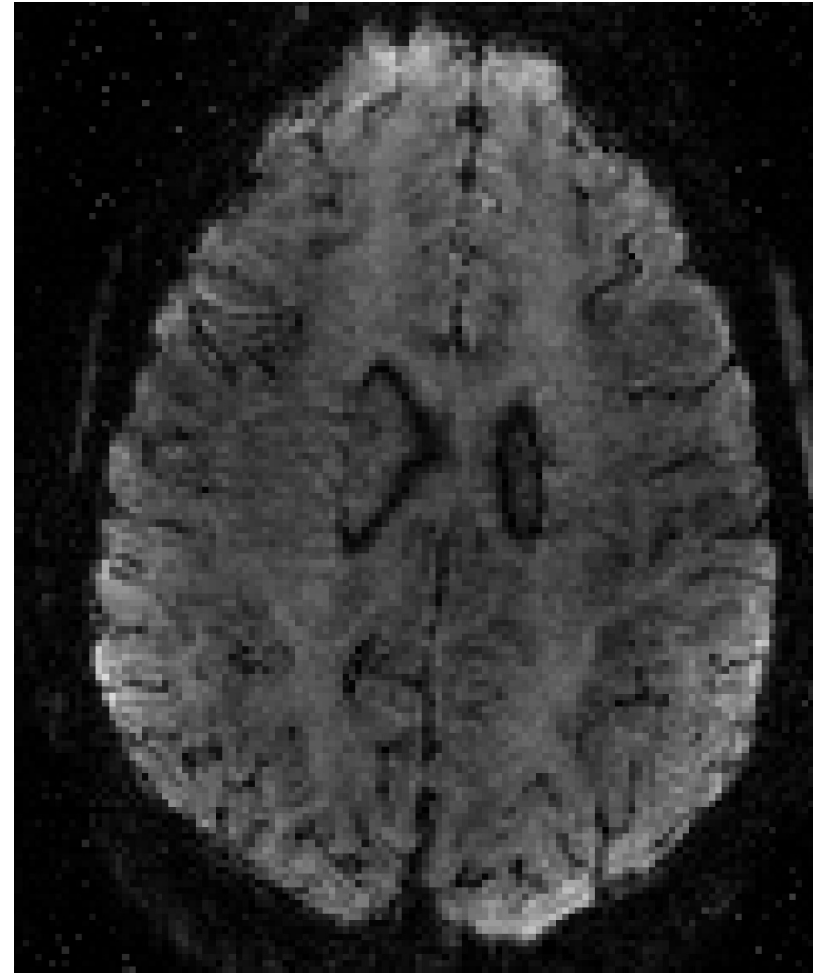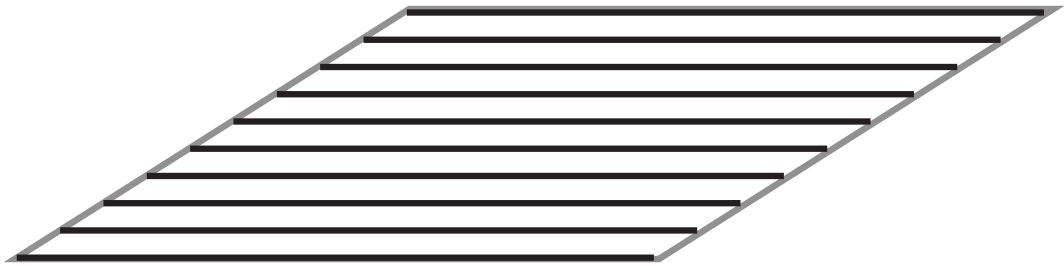

FLASH GRAPPA for fMRI: Talagala et al., 20015 MRM
FLEET GRAPPA for fMRI: Polimeni et al., 2016 MRM
dual polarity GRAPPA for fMRI: Hoge et al., 2016 MRM

Fat ghosts: small signal but large instability

Mean signal with normal fat saturation

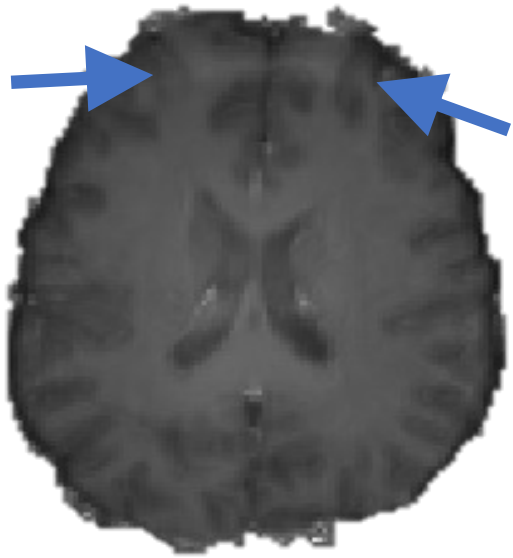


Standard deviation with normal fat saturation



Mean signal with ultra strong fat saturation




Standard deviation with ultra strong fat saturation

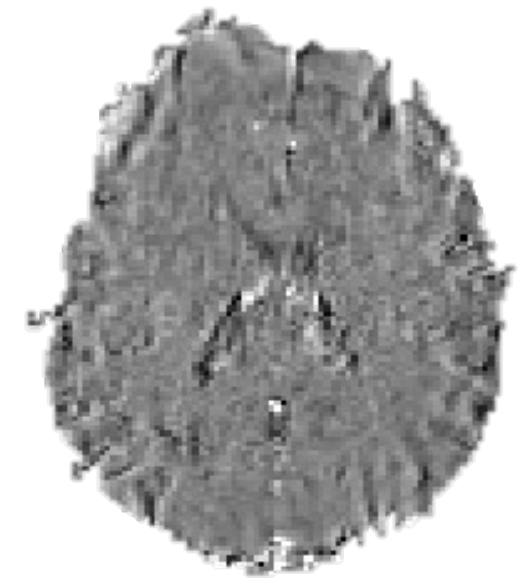

SMS and (task-induced) motion

2D-SMS-EPI

spatially neighboring
slices are acquired
distant in time

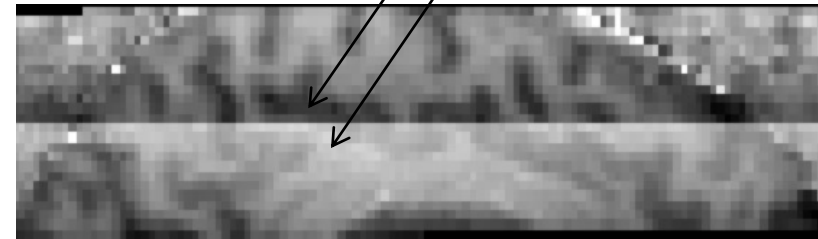

SMS and (task-induced) motion

2D-SMS-EPI



spatially neighboring
slices are acquired
distant in time





SMS and (task-induced) motion

2D-SMS-EPI

spatially neighboring slices are acquired distant in time

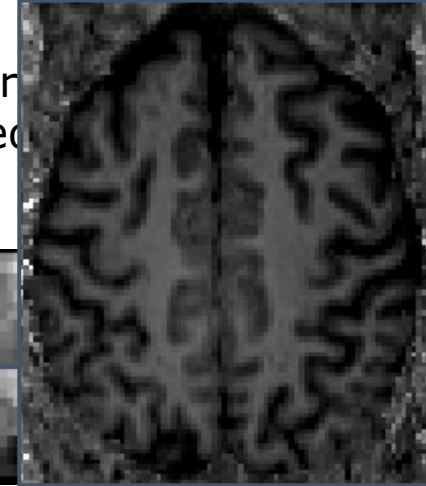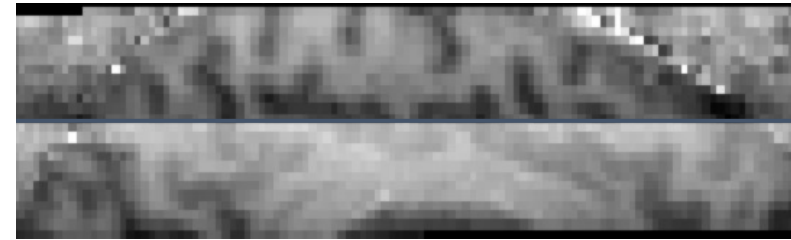

after motion correction

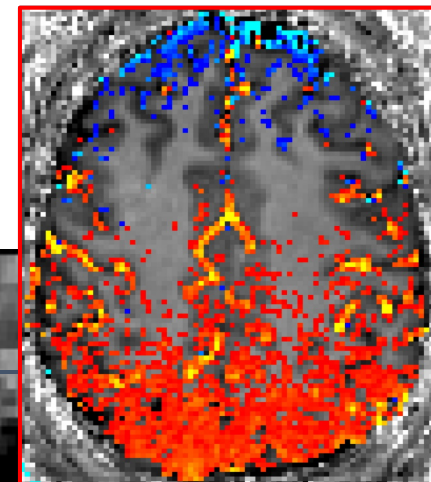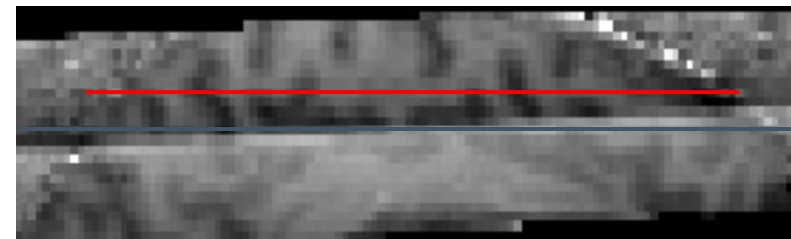

SMS and (task-induced) motion

3D-EPI



all slices are
acquired
simultaneously





[Poser et al., NeuroImage , 2010]

2D-SMS-EPI

spatially neighbor
slices are acquired
distant in time

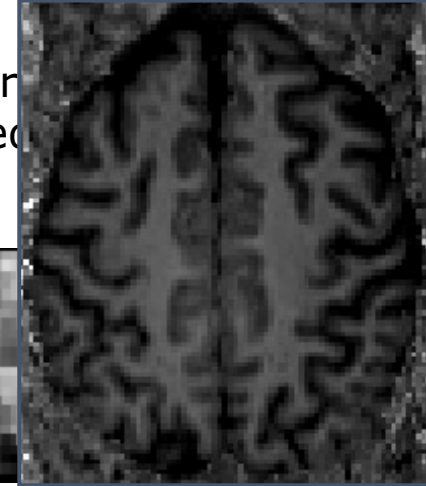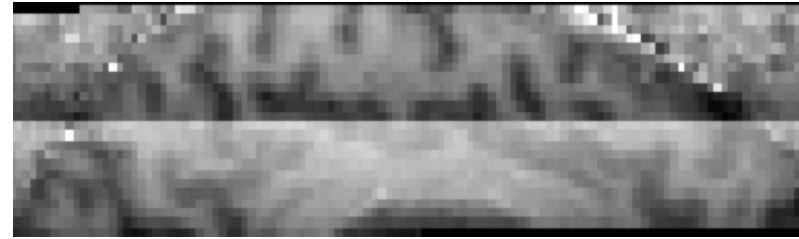

after motion correction

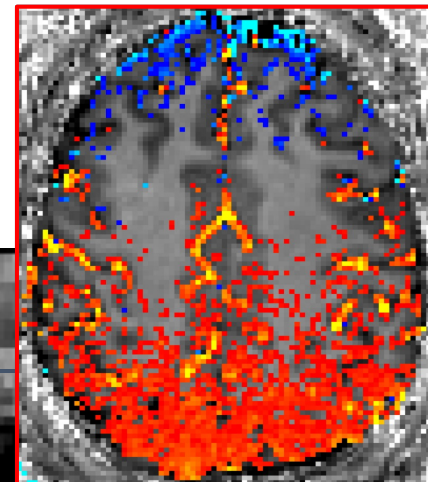
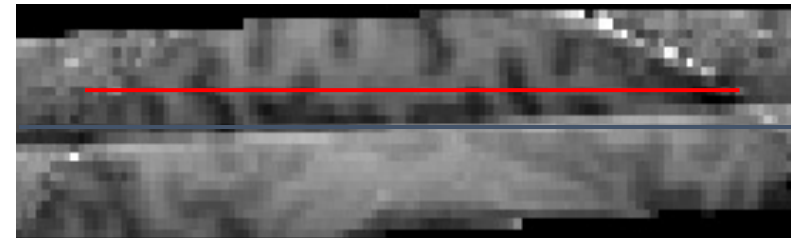


-3 Δ CBV ml/100ml 5

SMS and (task-induced) motion



3D-EPI

all slices are acquired simultaneously

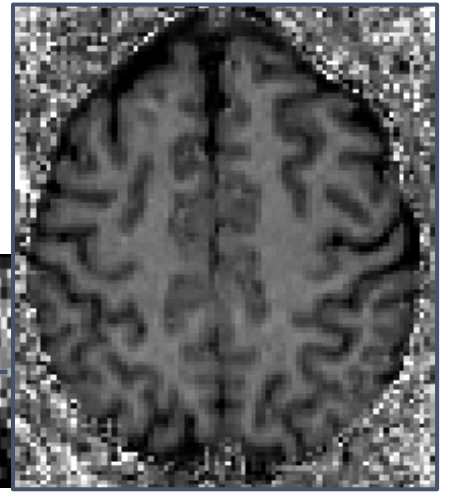
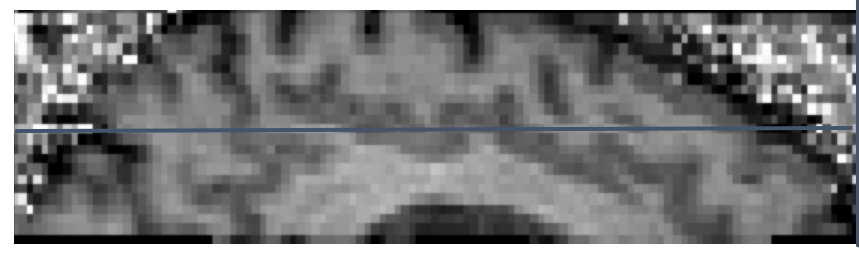


2D-SMS-EPI



spatially neighboring slices are acquired distant in time

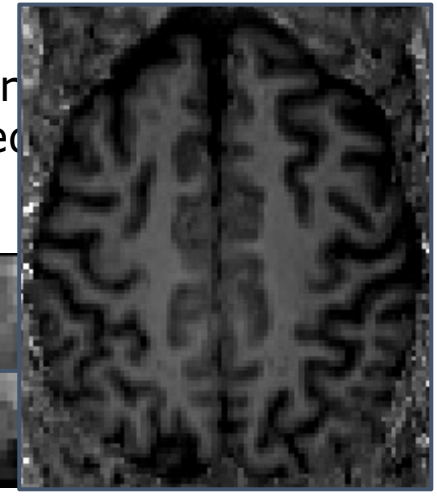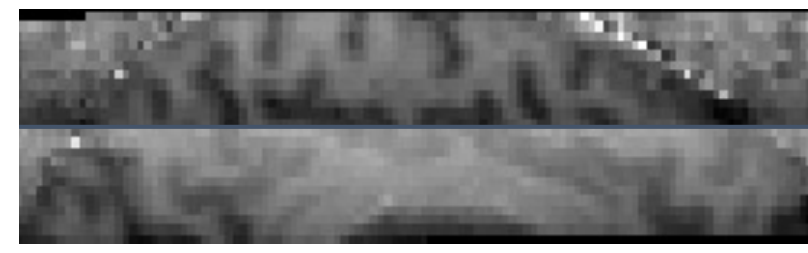


after motion correction

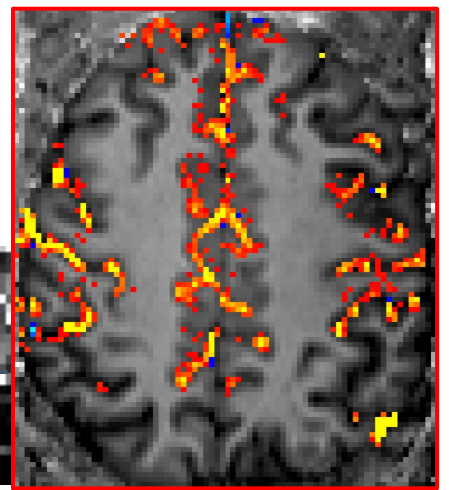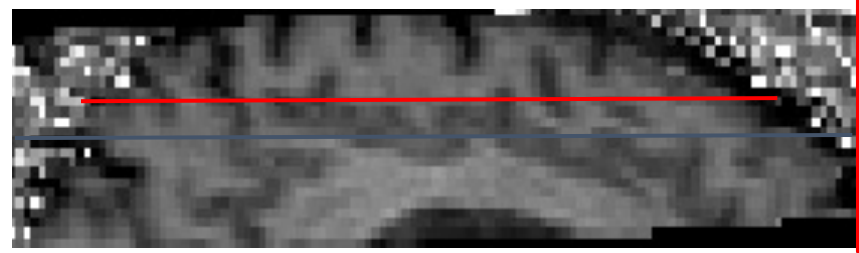

after motion correction

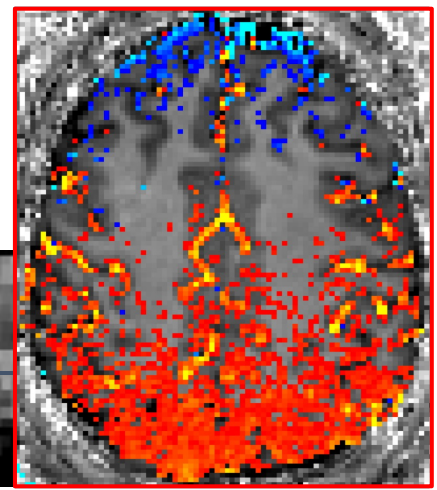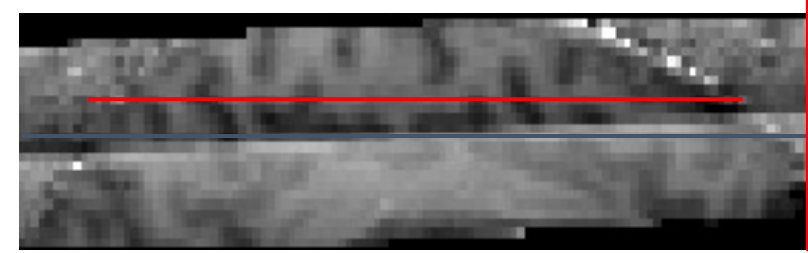

The "best" pulse sequence interacts with voxel size & SNR

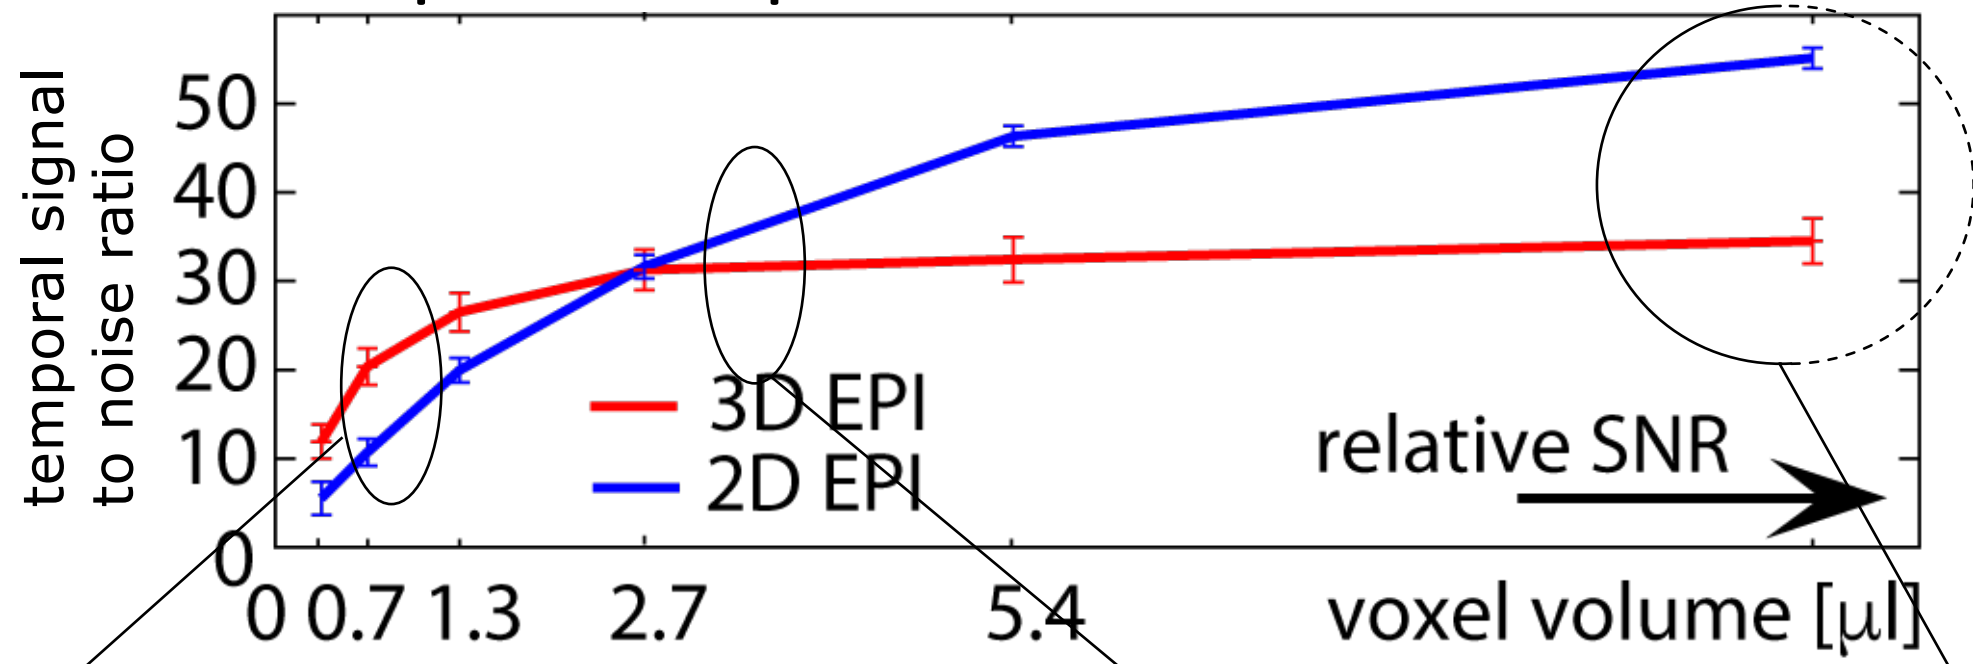


Huber et al.,
NeuroImage, 2016

relative SNR \rightarrow


SMS wins in physiological noise dominated regime

3D EPI

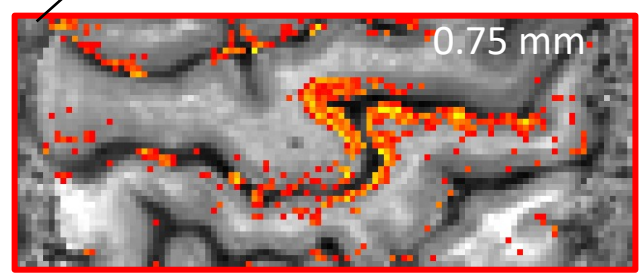



SMS is challenged in thermal noise dominated regime]

2D SMS


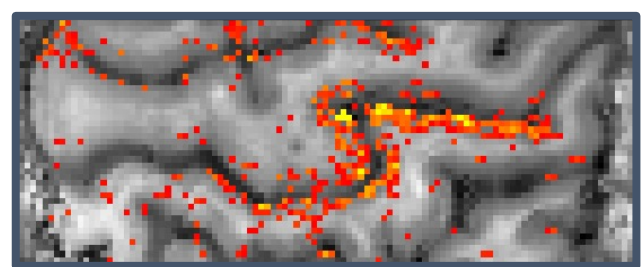


see poster #3605





1.5 mm

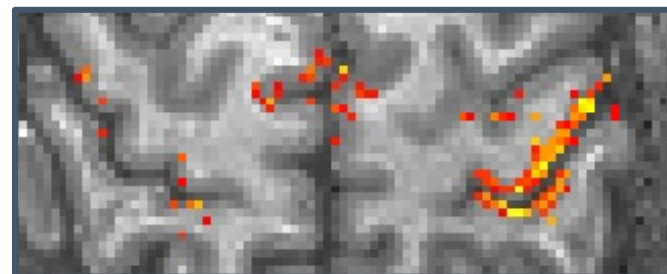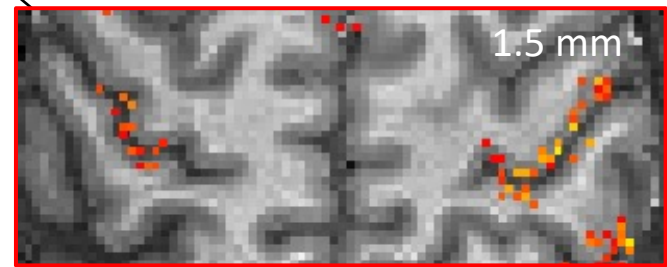

3 mm

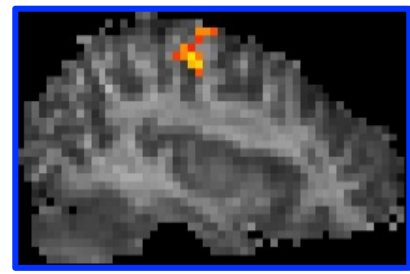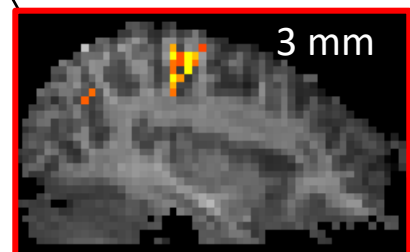


Pulse sequences contrasts

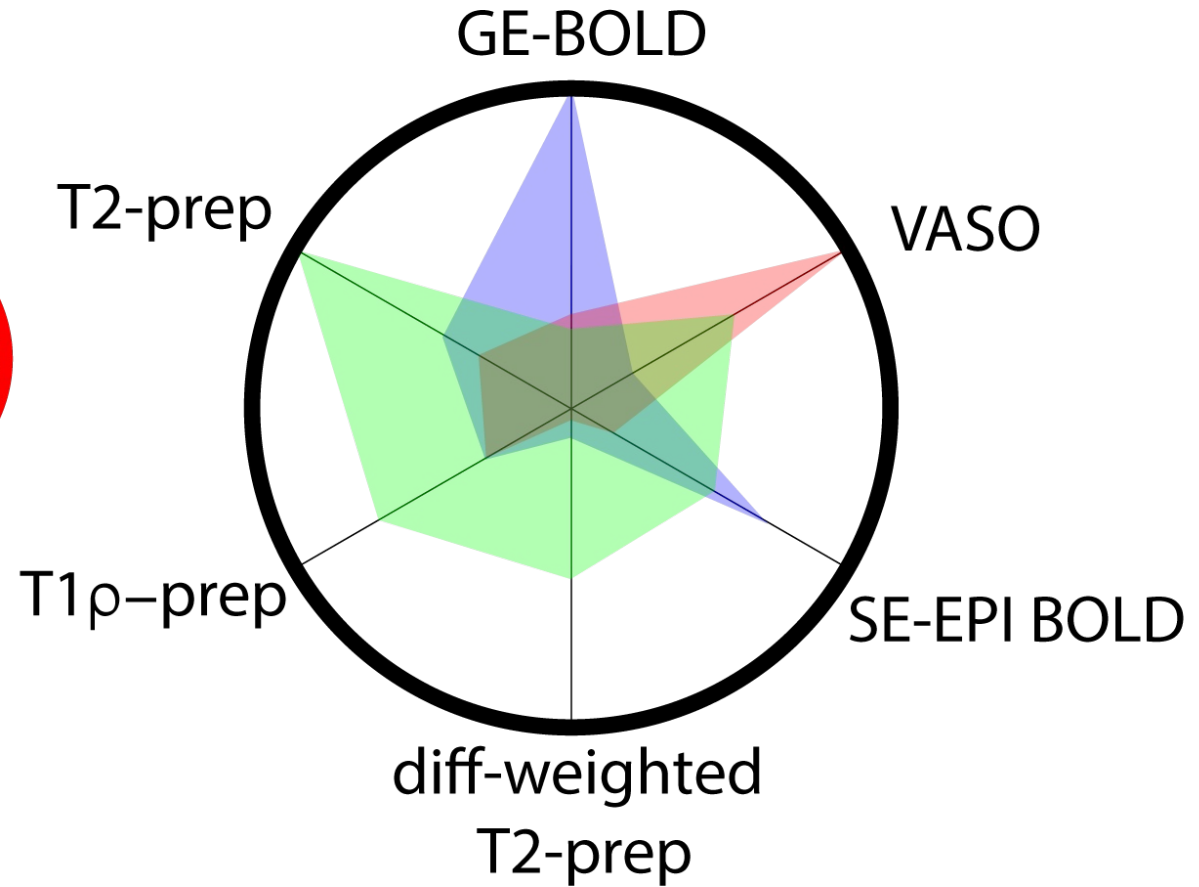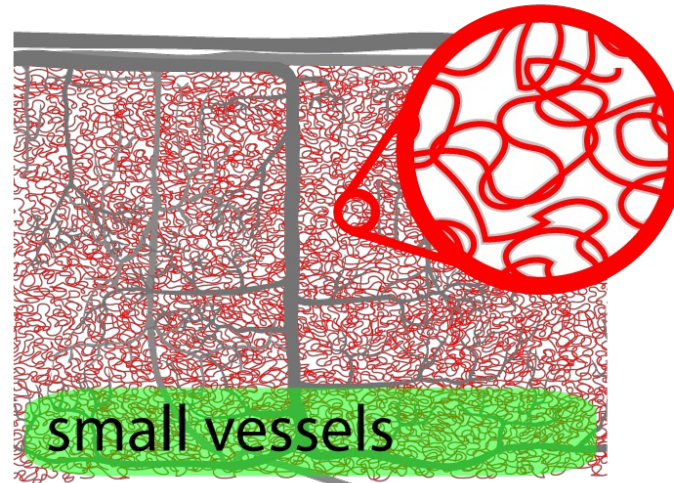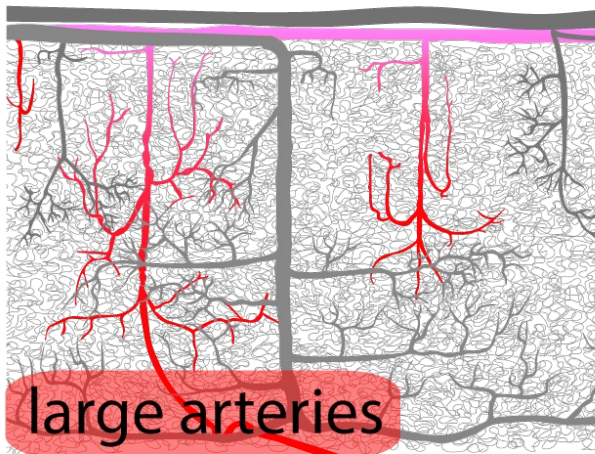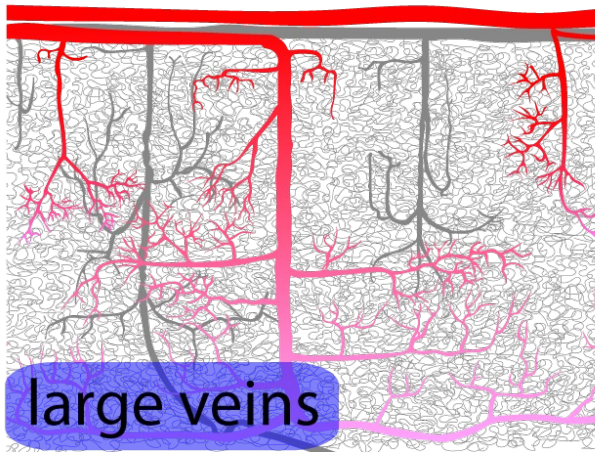



Images from Laurentius Huber
 graphical depiction of review articles [Uludağ and Blinder 2017] and [Huber et al., 2017]
 drawn based on Duvernoy, 1981 Brain Res

Parameters and Pulse Sequences


Example 5 MRI contrast

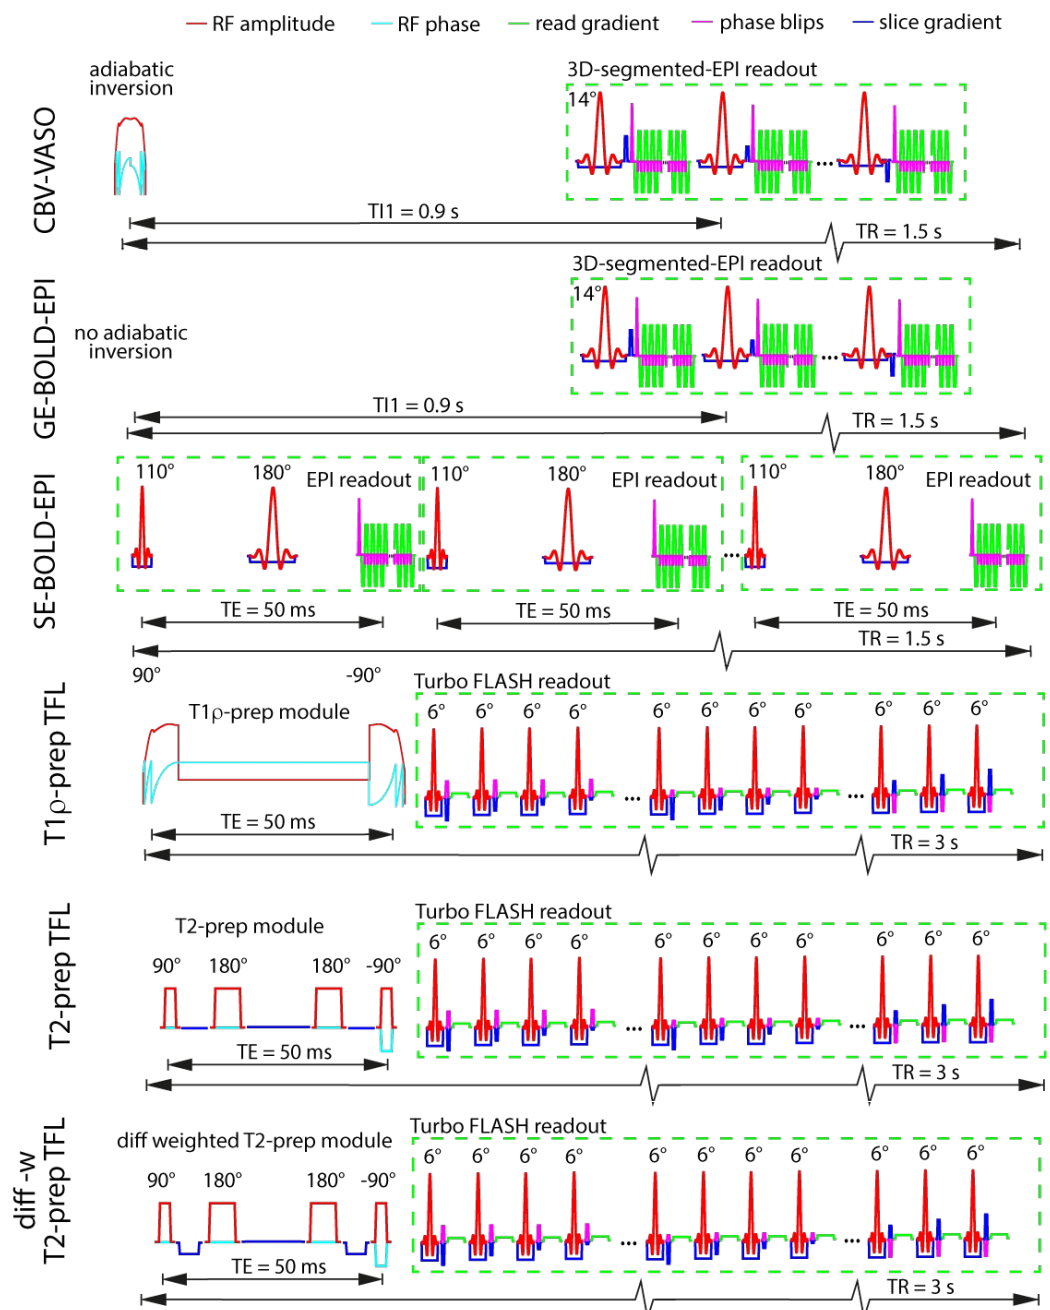


[Lu, 2003]
[Huber, 2014]

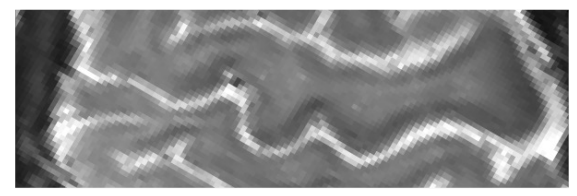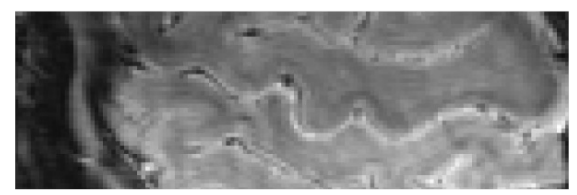

CMRR C2P
[Auerbach, 2013]

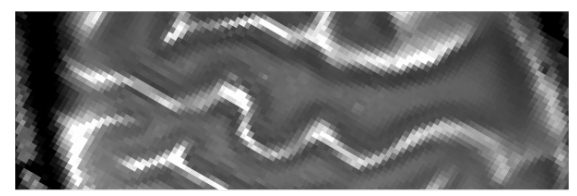

[Rane, 2013]

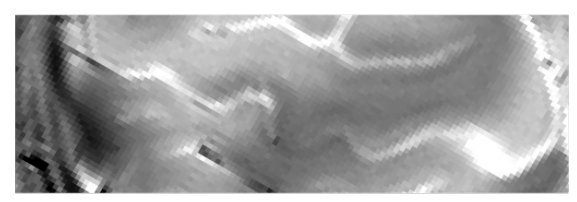


[Hua, 2014]




[Duong, 2003]
Images from Laurientius Huber

[Huber et al., ISMRM, 2017]

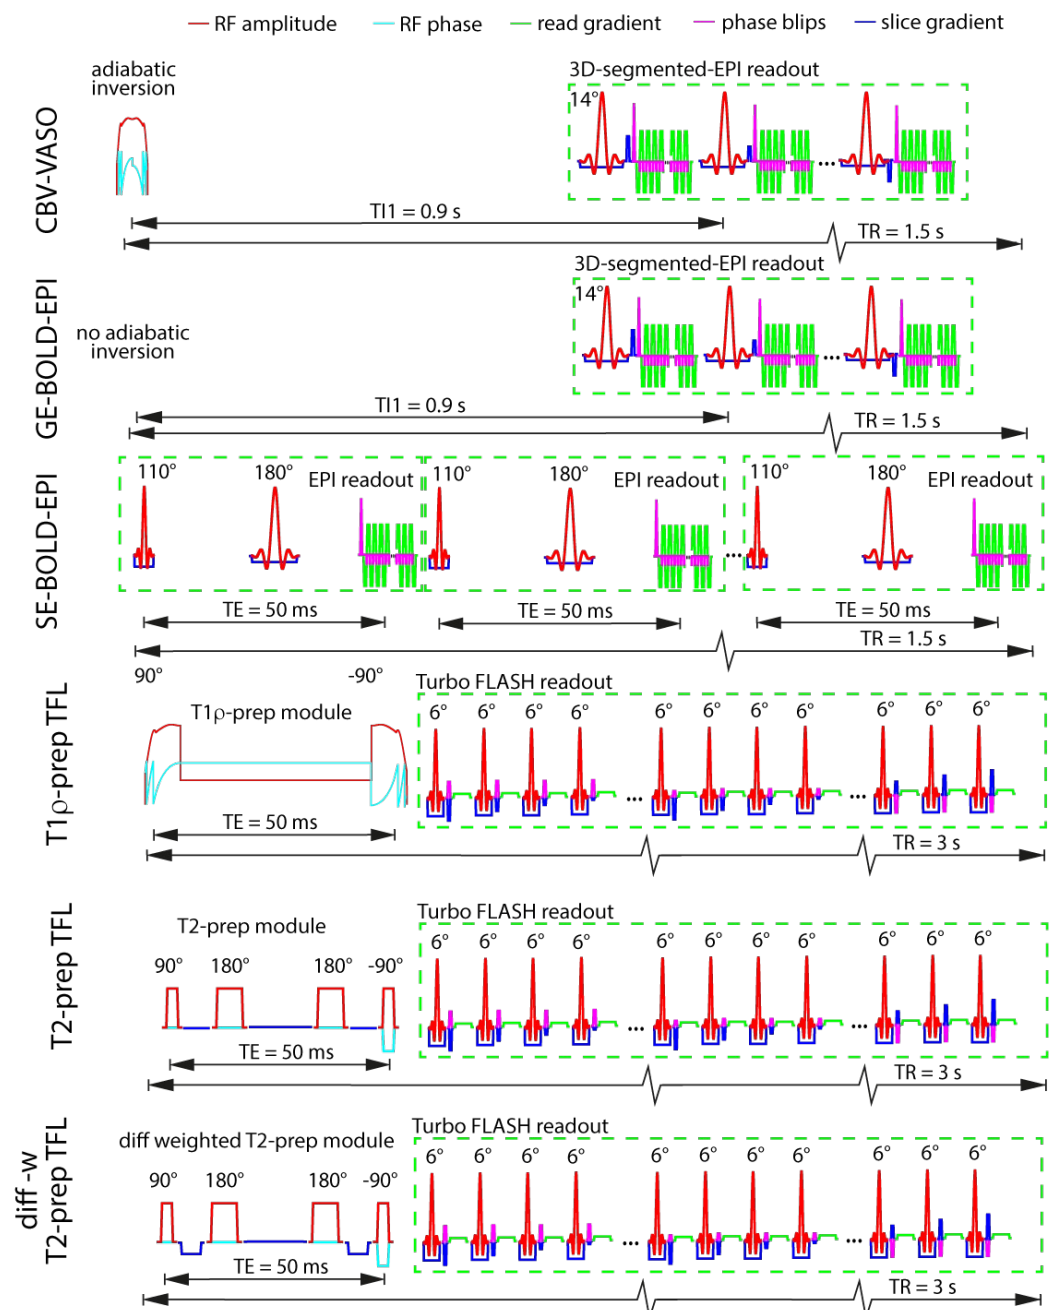


Functional Response

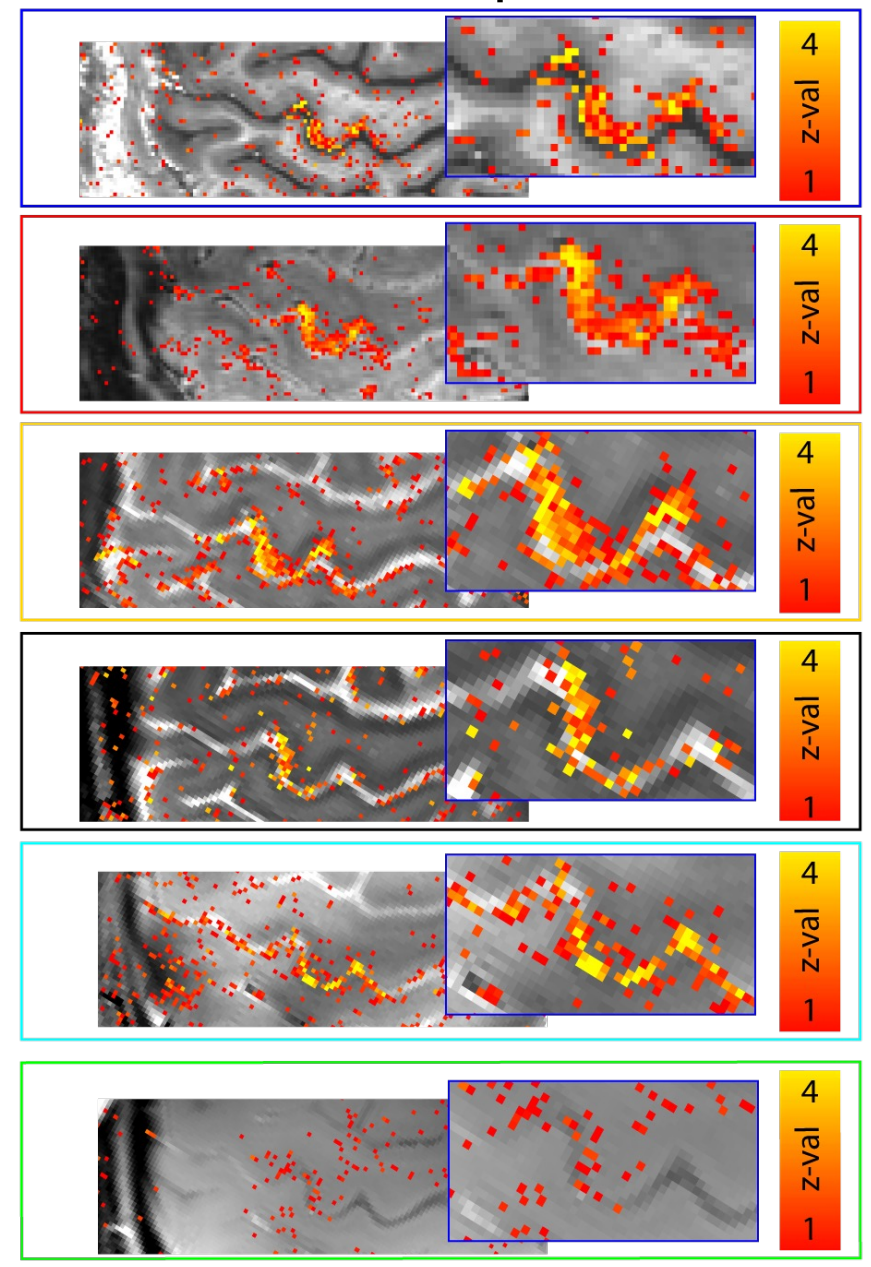


Parameters and Pulse Sequences

Example 5

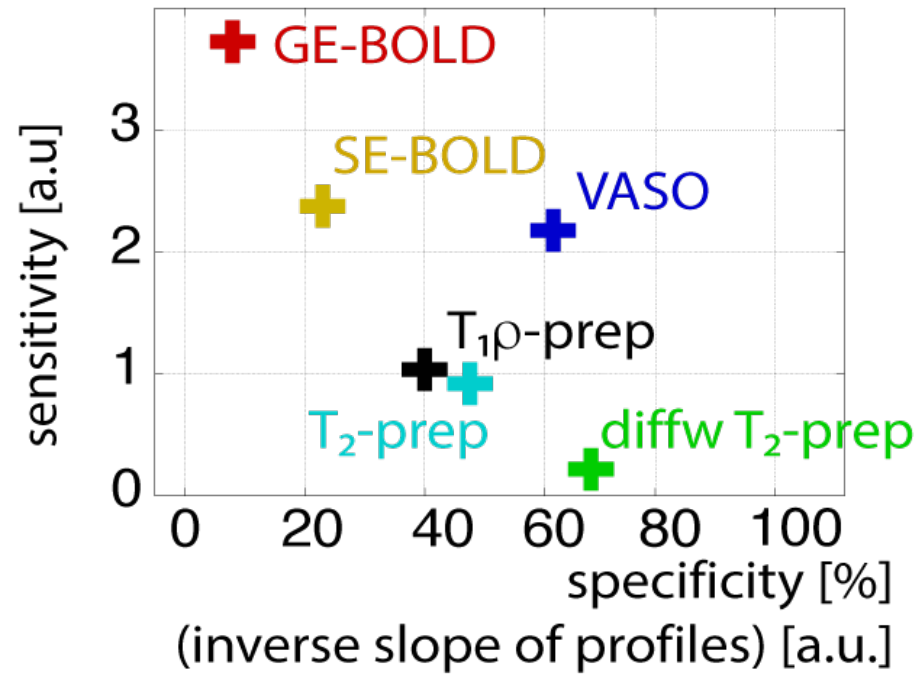


- VASO
- $T_1\rho$ -prep
- GE-BOLD
- diffw T_2 -prep
- SE-BOLD
- T_2 -prep


Functional Response

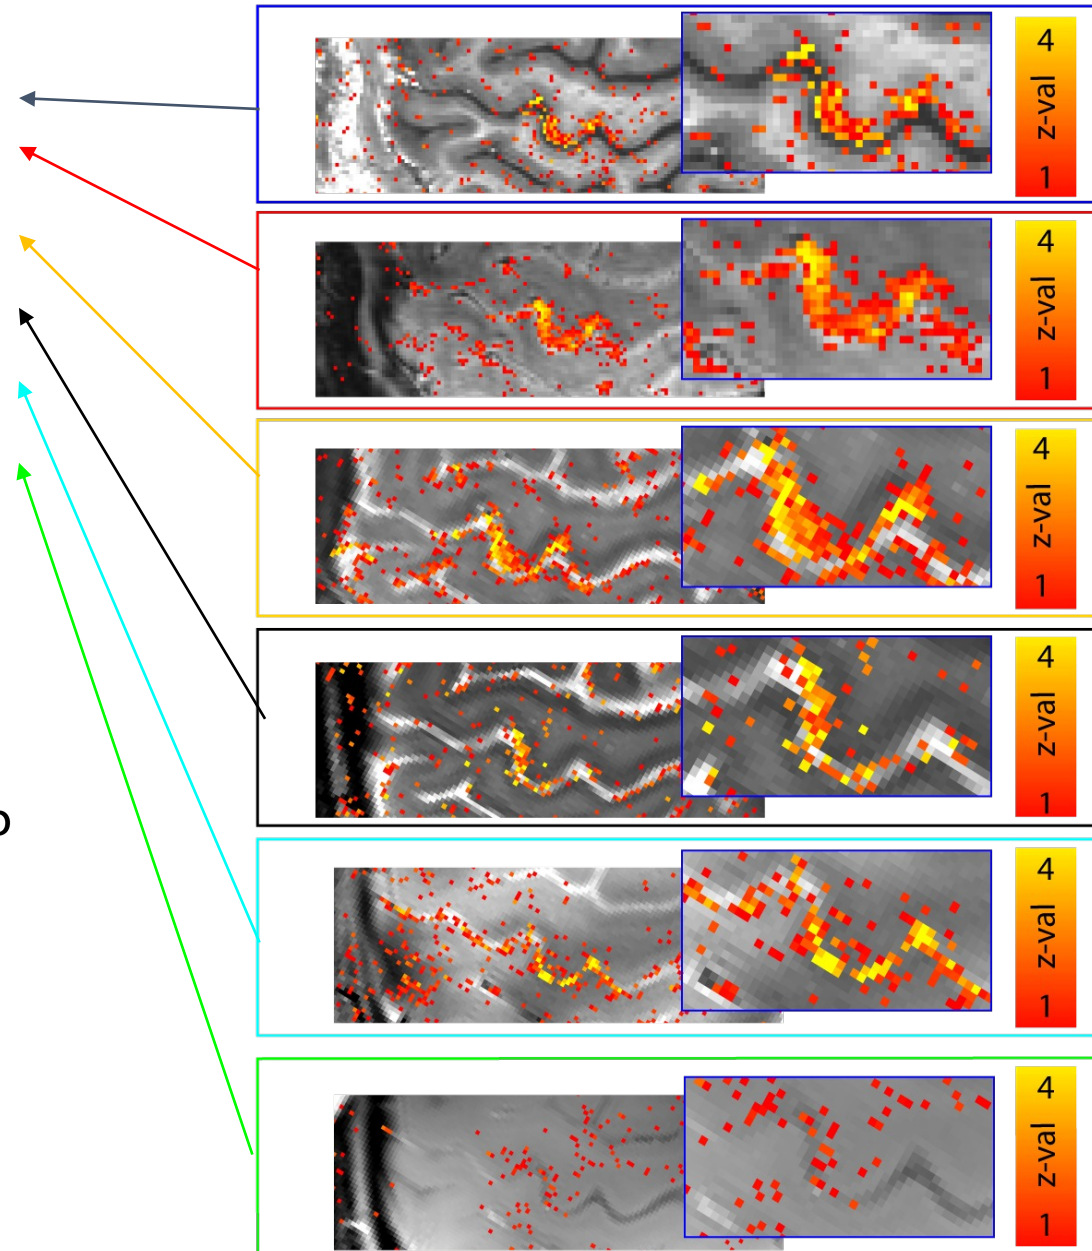

Real time motion correction during data collection

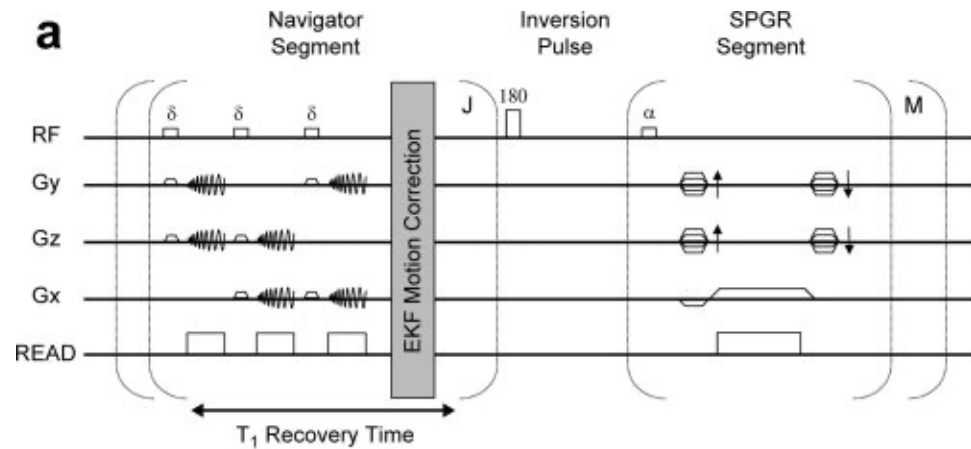

MPRAGE anatomical image

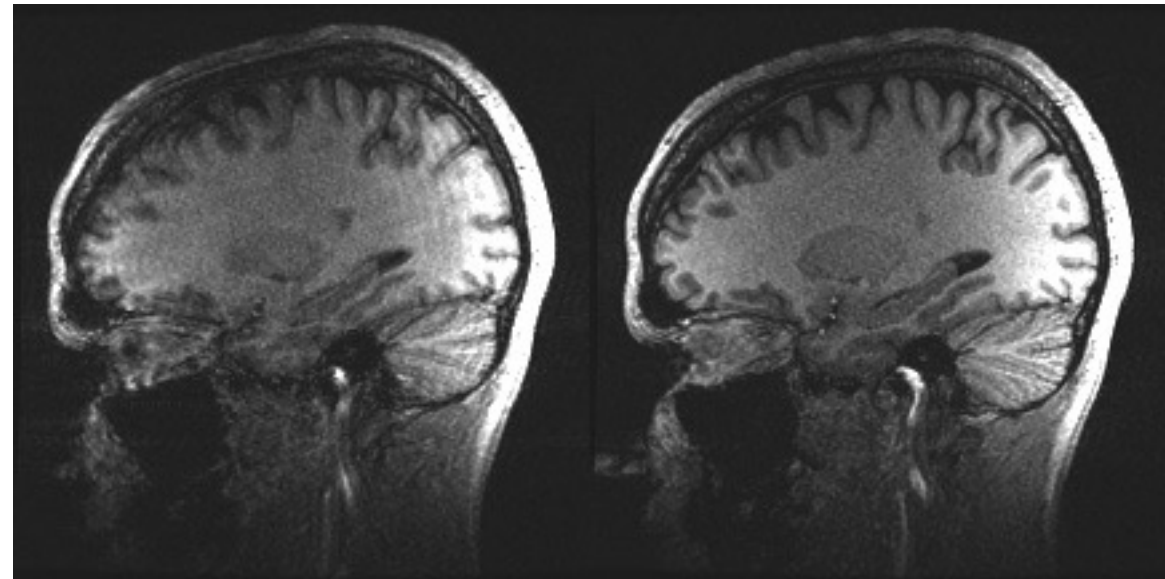


Without PROMO

With PROMO

Calibration or Baseline scans

Collecting an additional scan that helps correct for subject-specific systematic variation

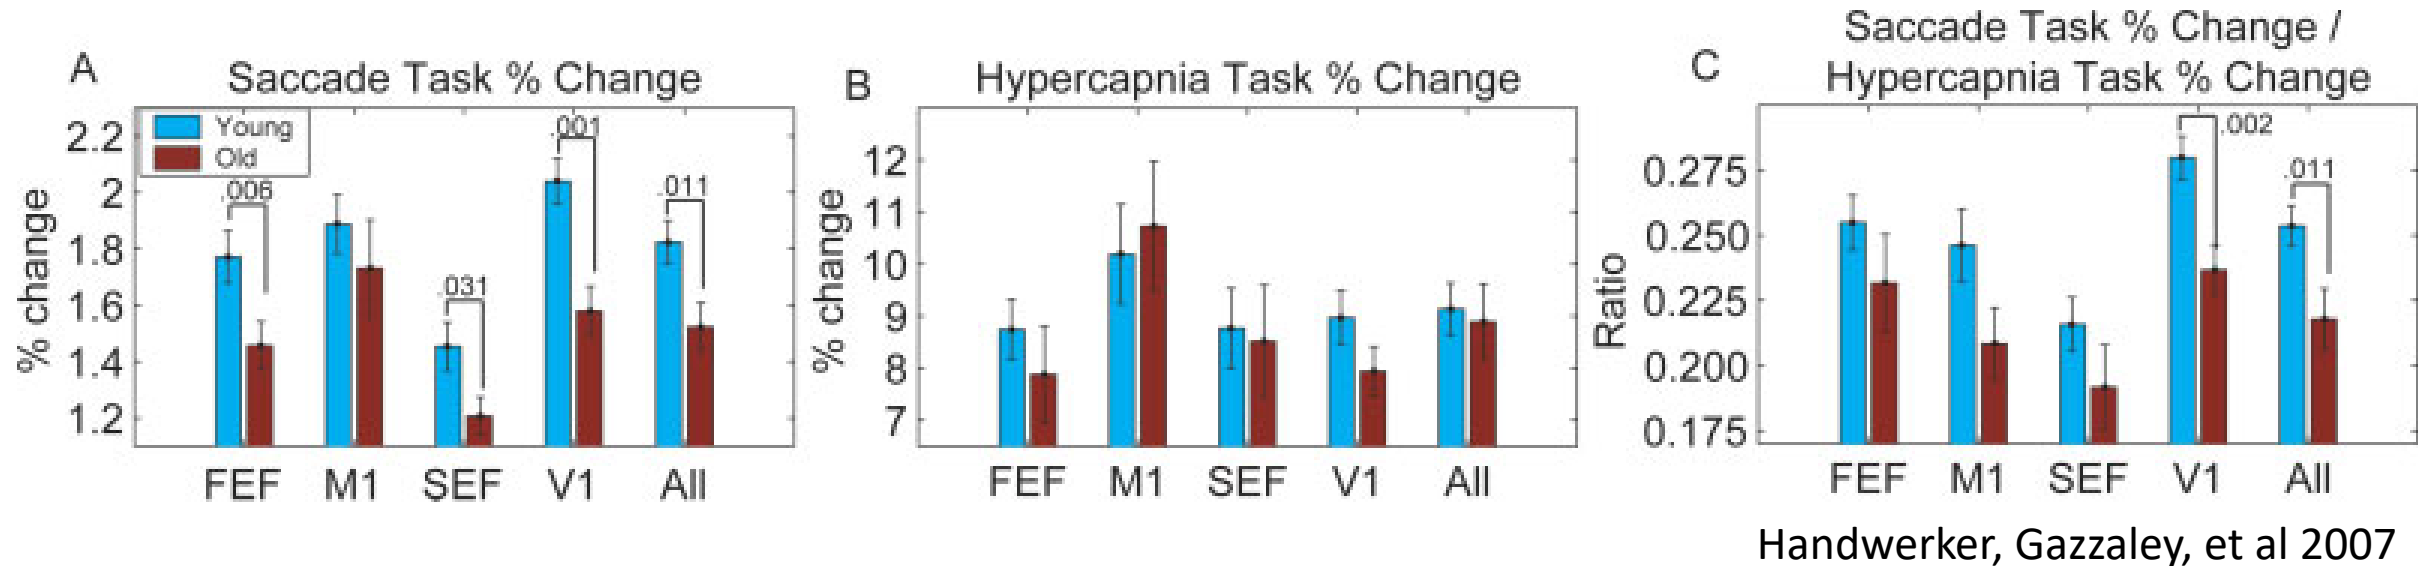

- Other examples are simple tasks, enriched gas breathing, baseline CBF, standard deviation of resting scans
- Good sanity checks and may be useful
- These can take scanner time away from studying the effects of interest, which has limited their popularity
 - Relatively few clinically interesting studies use them


Peripherals and Participants

- Peripherals
 - Respiration, Pulse, Peripheral NIRS
 - Eye movement
 - Head movement
 - Multimodal neural measures: EEG, optical, Galvanic skin response
- Participants
 - Head restraints
 - Good instructions, training, & feedback
 - Good task design & response monitoring

Collect respiration & pulse data

- Removal of physiological noise during post processing is nice
 - RETROICOR (Glover, Li, Ress 2000)
 - Respiration Volume / Time (RVT) (Birn, Diamond et al 2006)
 - Heart rate (Chang, Metzger, et al 2013)

- **Knowing what your volunteer is doing is essential**

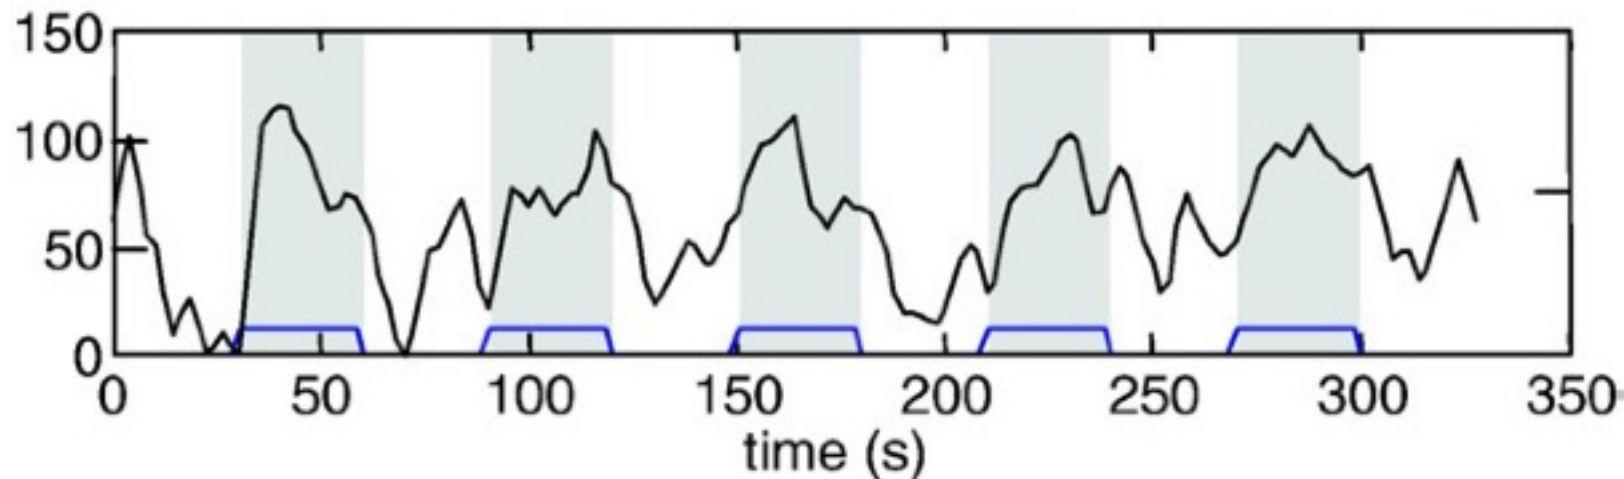


RVT (black).
Word/nonword task
block design (blue)

Collect respiration & pulse data


A minor confession

Present a 200ms flickering checkerboard every 18-24s

Volunteers press a button and move their eyes

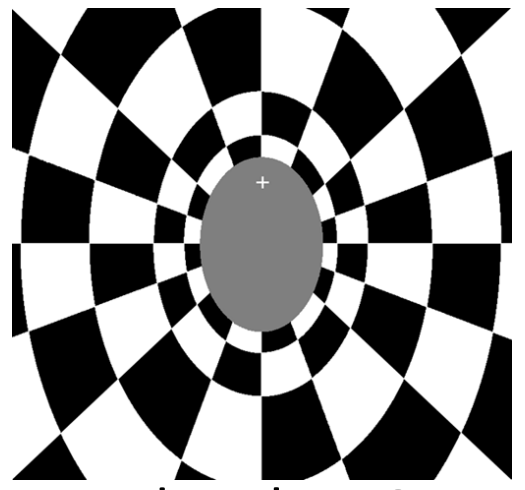

Handwerker, Gazzaley, et al 2007

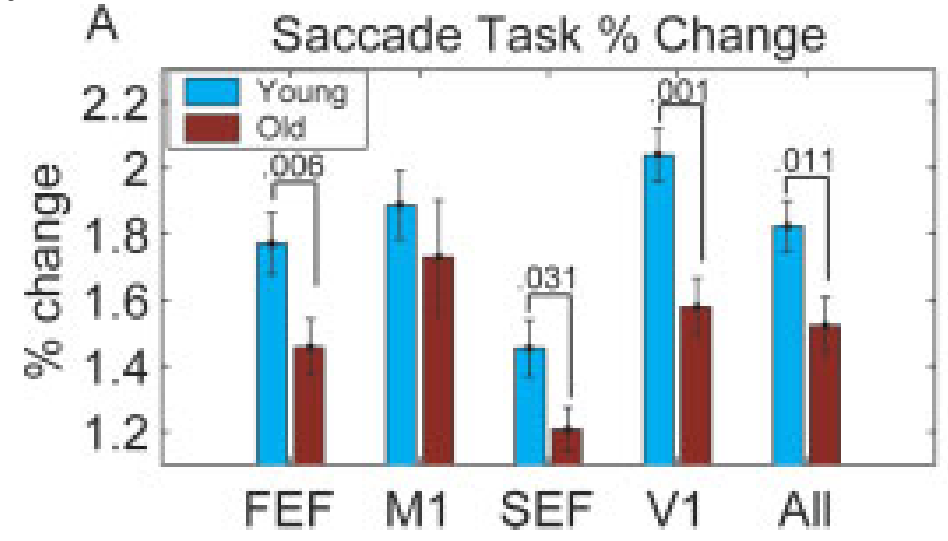


THE UNPUBLISHED PART

- Stimuli presented for 3s, 6s & 12s durations to examine response scaling across populations
- A non-trivial # of volunteers held their breath for whatever the hold duration was
- If I hadn't collected respiration data, I would have published a visually appealing results that were severely confounded by task-locked breath holds
- How many studies with variable task durations recorded respiration traces???


Collect respiration & pulse data

Respiration can really mess up your data

Flickering Checkerboard

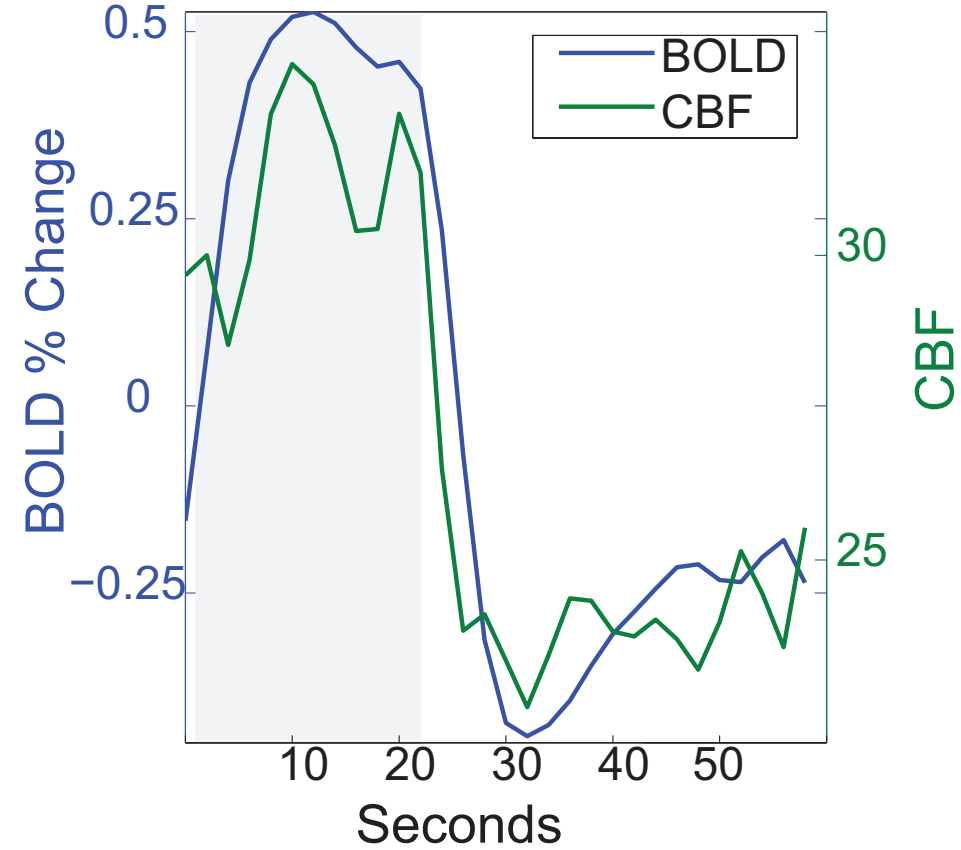


20sec Breath Hold

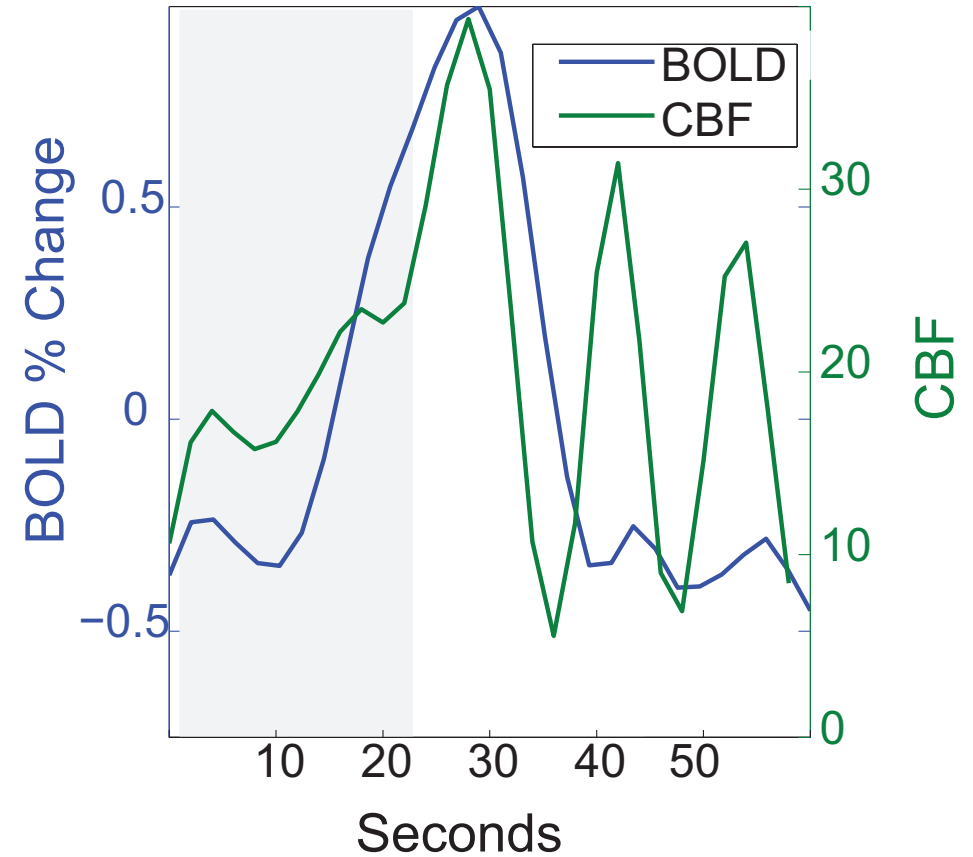


Collect respiration & pulse data

Respiration can really mess up your data



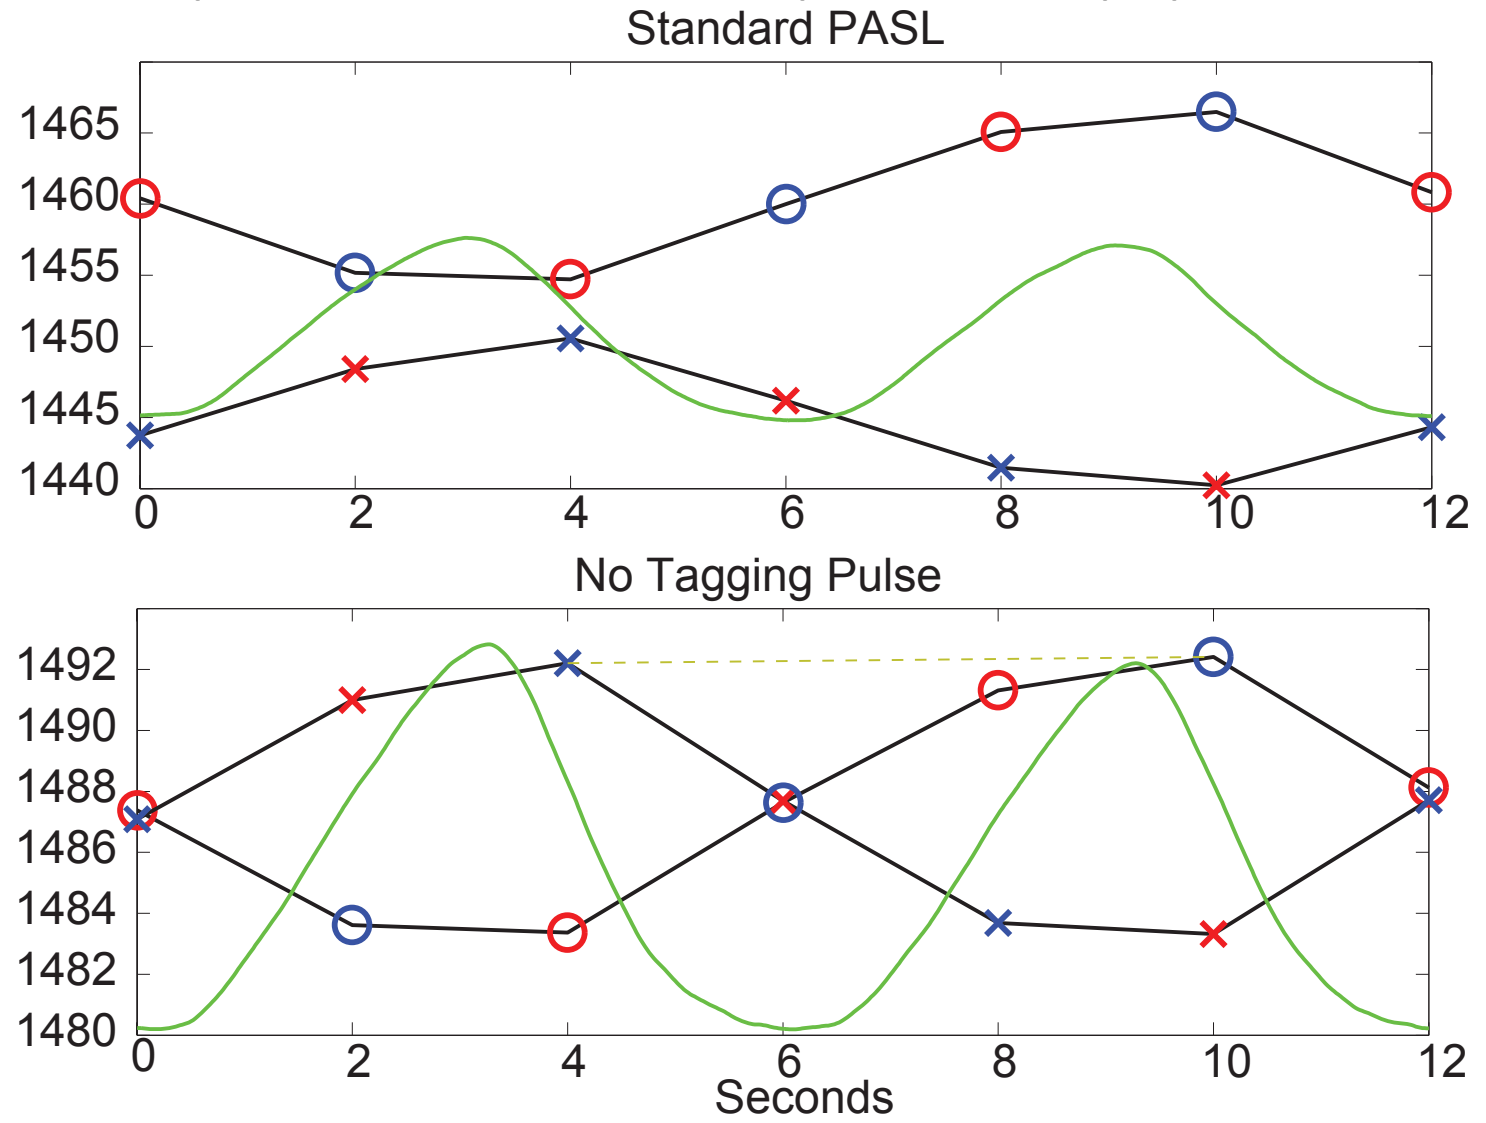


ADVICE FOR collecting respiration & pulse data


- If you want to use post-processing removal methods, make sure respiration and cardiac traces are connected to MRI acquisition times
- For respiration: To conduct an RVT correction, make sure the response magnitude doesn't auto-scale and you know the relationship between chest movement & signal
- For cardiac: Pulse oximeters are sensitive to finger movement. Take the time to make sure the oximeter is secure and tell the volunteer to minimize finger movement during a scan
- Monitor traces before & during scanning

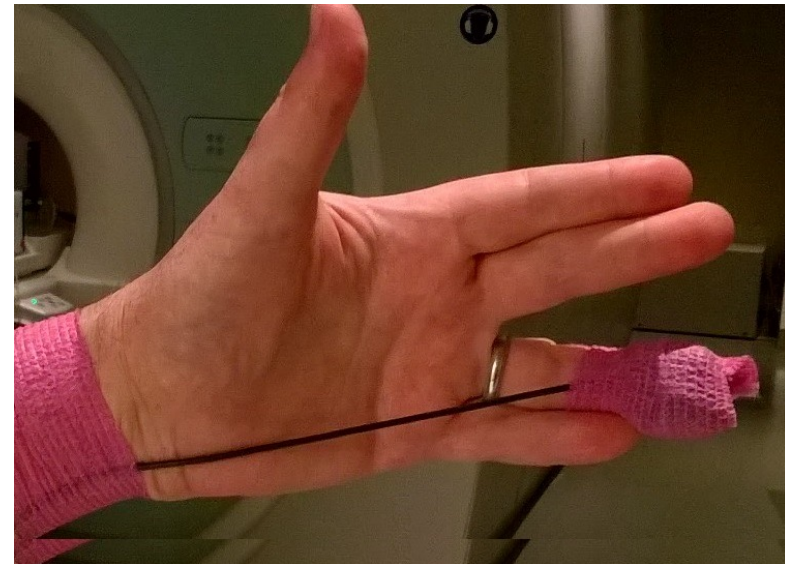


Peripheral near-infrared spectroscopy

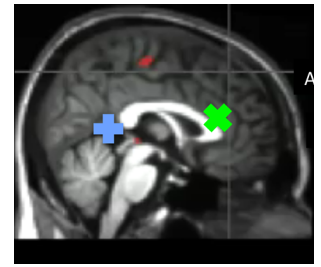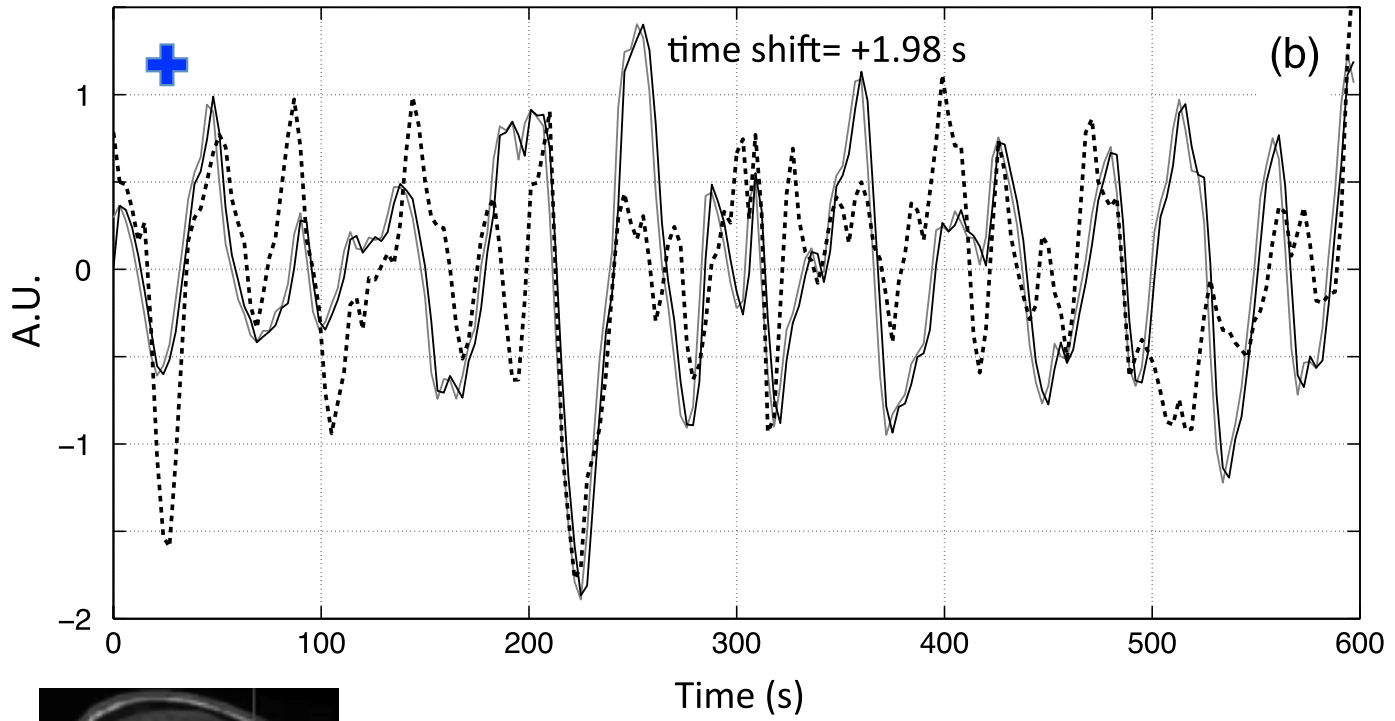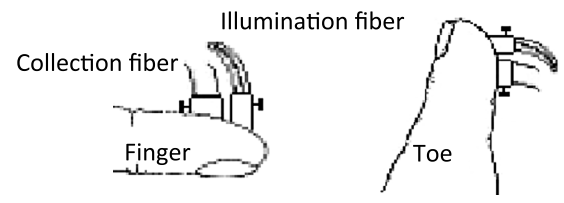

- BOLD from brain
- $\Delta[tHb]$ from finger
- $\Delta[tHb]$ from finger with time shift

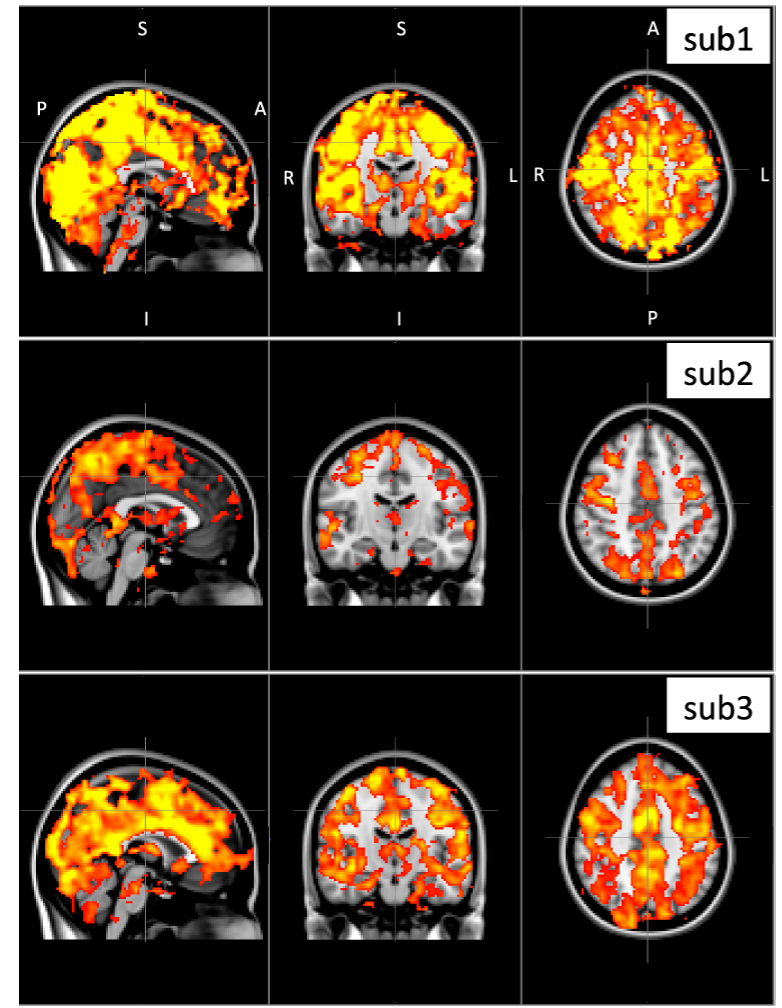

Eye tracking

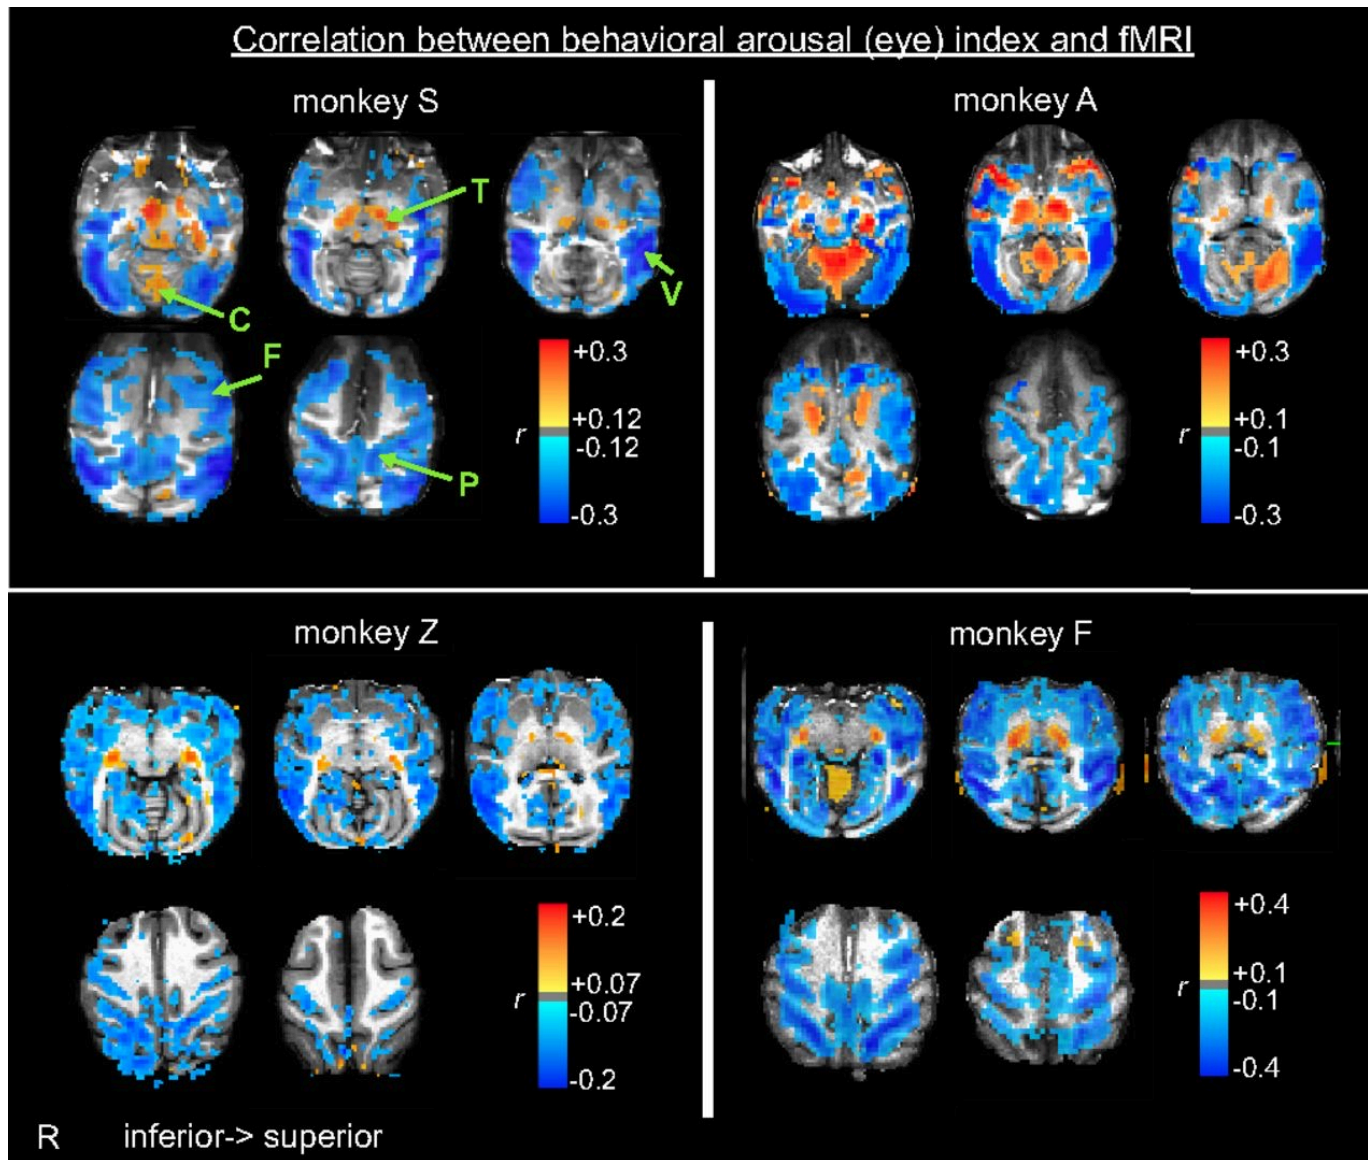


- Correlations to eyelids open vs closed
- Other studies have shown gaze to also be an arousal/attention measure
- This variation may have a neural origin, but it can still be noise when unmodeled

Head Movement

- Less head motion -> Less need to remove motion in data processing
- Head movement may systematically vary across populations
- Don't assume the way you saw someone else restrict head movement is the best way
 - “The best” varies by head coil, head size, & population
 - There are more and more options



<http://www.magmedix.com/pearltec-multipad-slim.html>

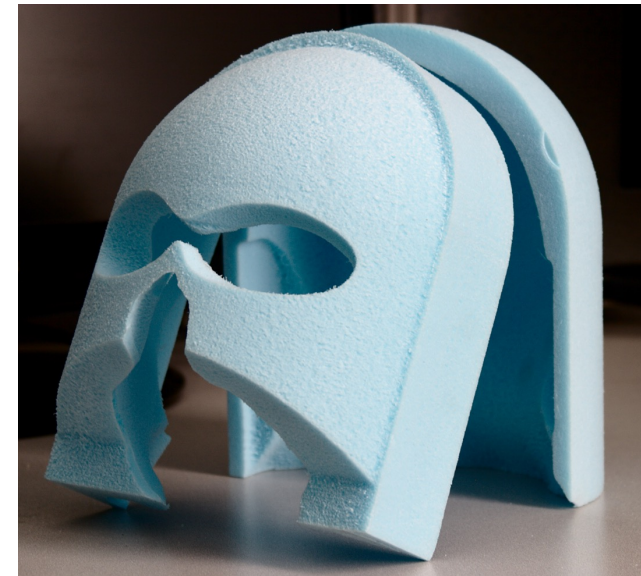


caseforge.co

Prepare participants

- Take the time to make sure a participant knows what to do in the MRI and is comfortable
- The more feedback you get in a task, the better you know what a participant is doing
 - For classic "resting state" scans, peripheral measurements are particularly useful
- Noise IS NOT independent from task design

Head Movement


Experimental design affects head motion

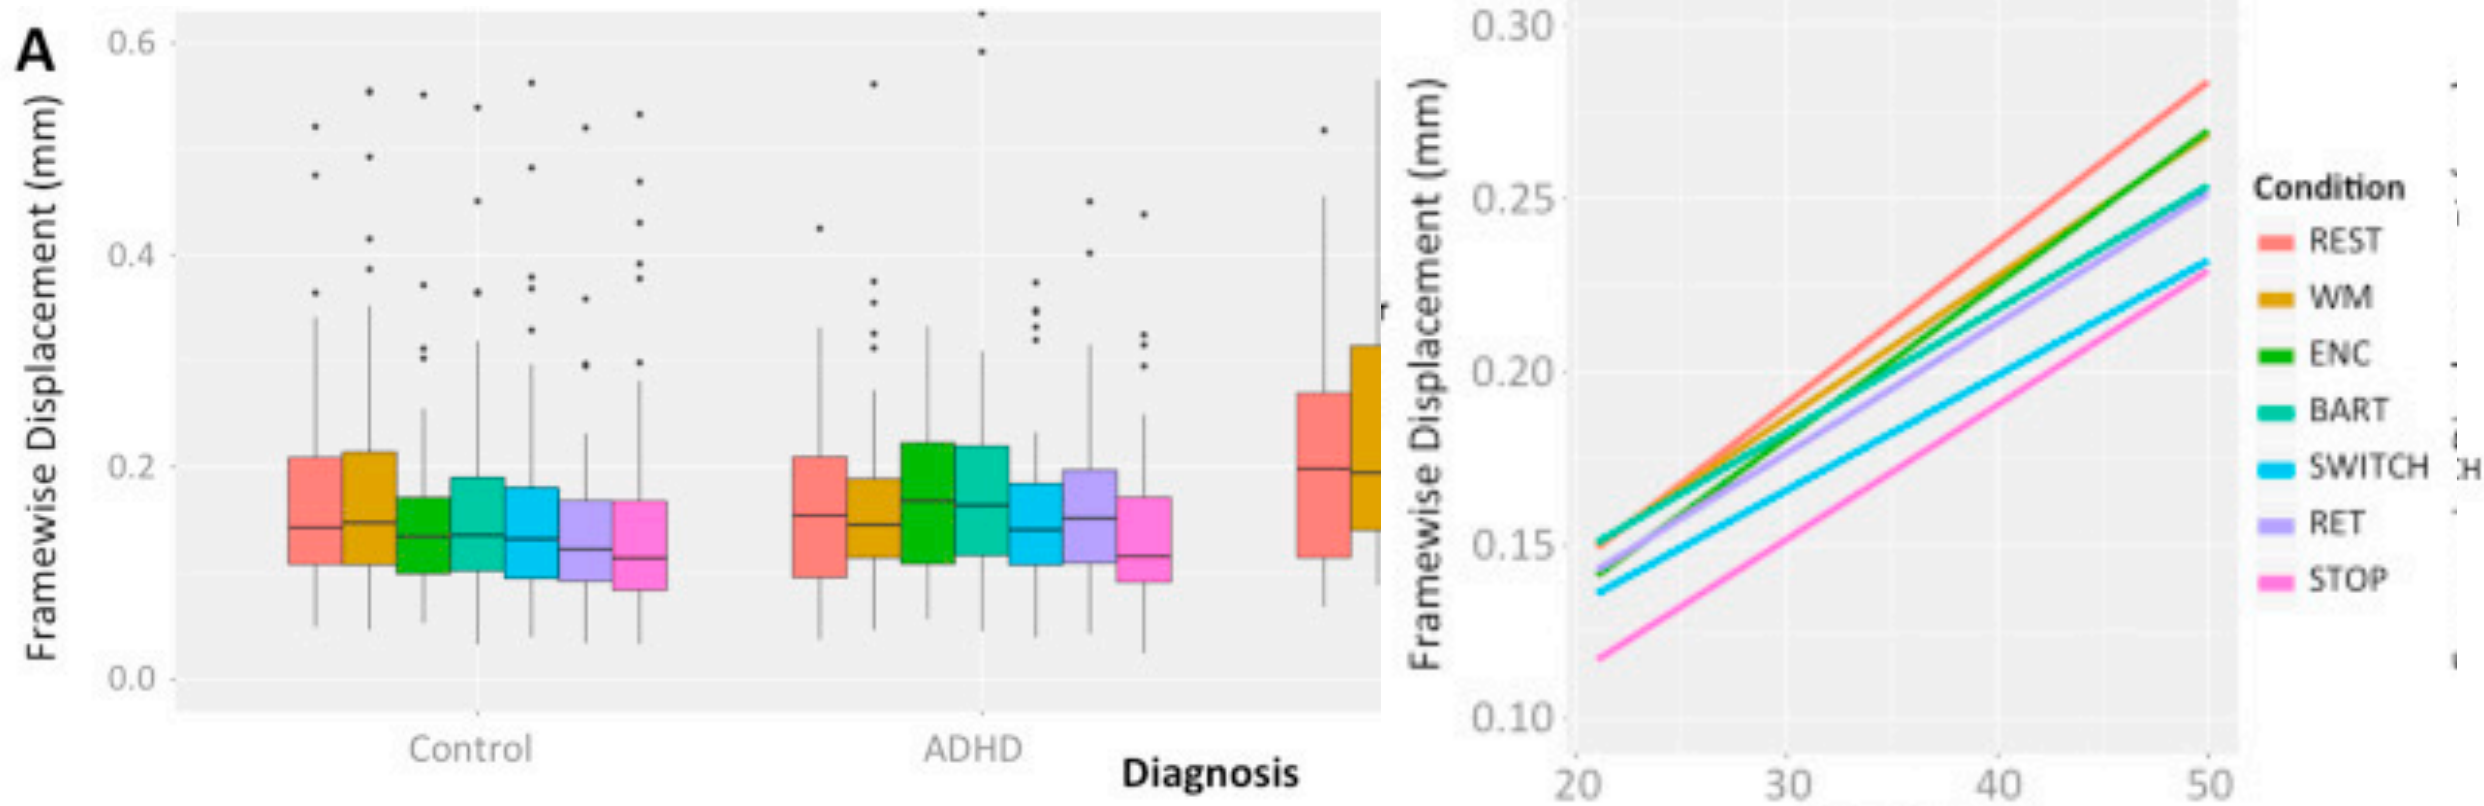

Huijbers, Van Dijk, et al 2017

Head Movement

Experimental design affects head motion

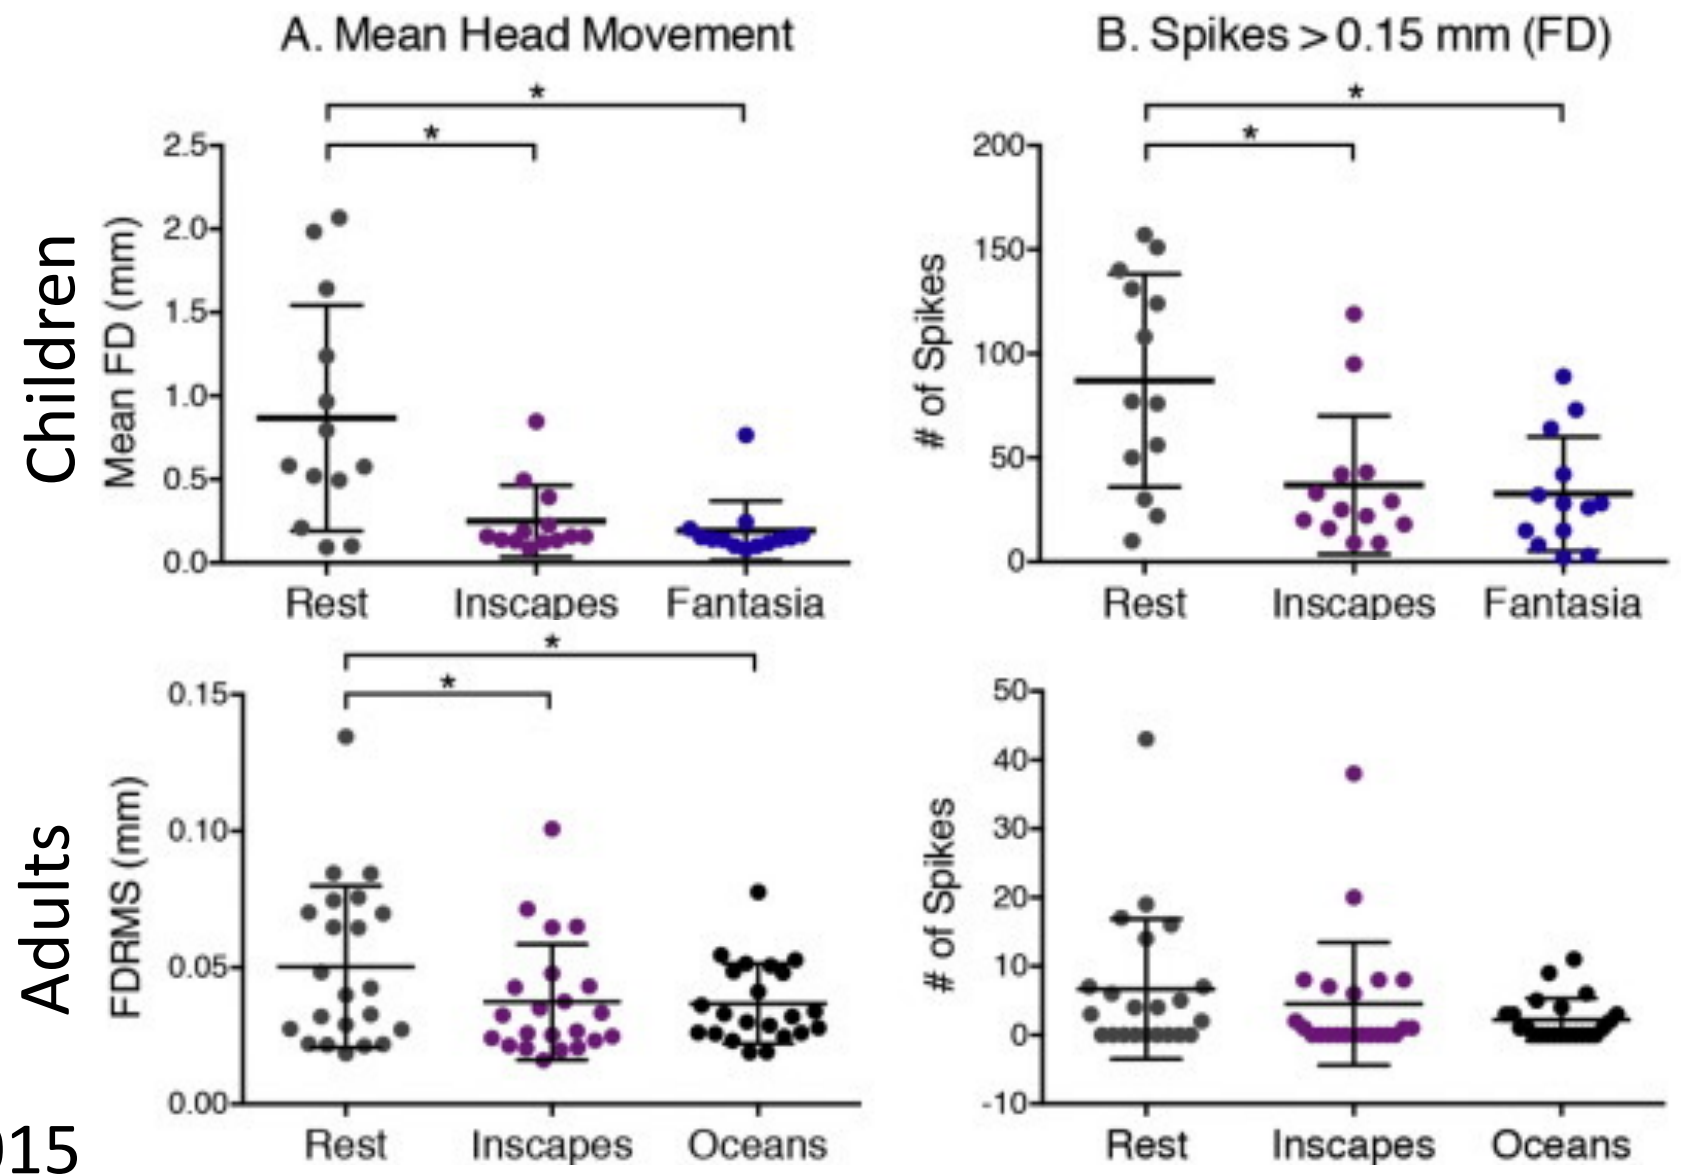

Preventative scanner health

- Regular Quality Assessment (QA) scans
- Regular Overall Evaluation of Results
- Real Time Data Observation


Quality Assessment Scans

NIH Intramural example


- Approximately daily scans of an oil phantom for every commonly used head coil on every scanner
- Parameters that can provide long-term consistency
 - Single Echo EPI, no acceleration; 72x72 grid; 37 slices; 3mm³ voxels; 5-10 min of data per receiver coil
- Save reconstructed & (sometimes) raw data
- Try to automate processing & recording pipeline

Sample QA Plots of Temporal Signal To Noise Ratio

From different scanners

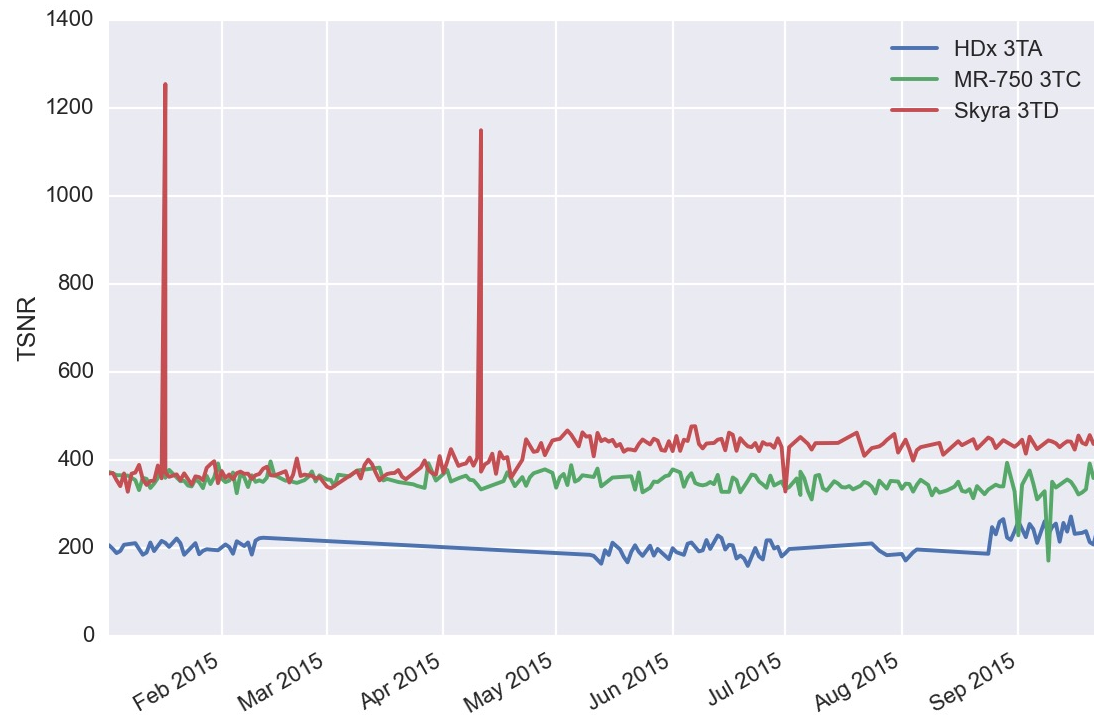

From each receiver coil on one scanner

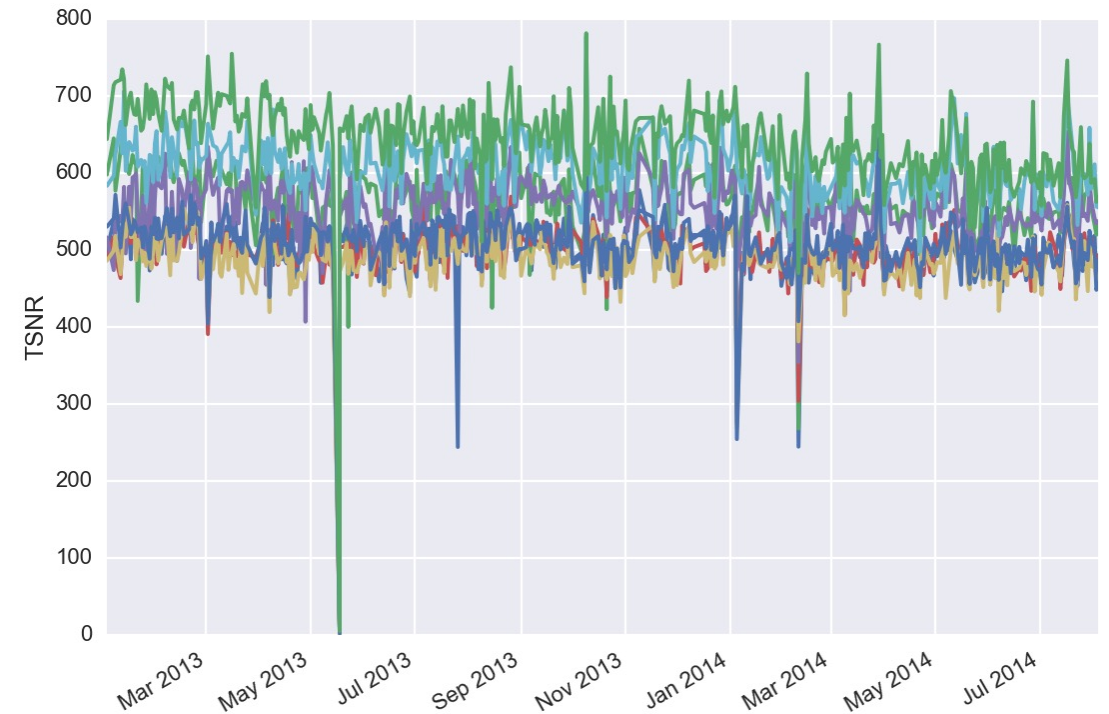

Regular Results Evaluations

MRIQC: group anatomical report

Summary

- Date and time: 2017-02-05, 12:27.
- MRIQC version: 0.9.0-rc2.


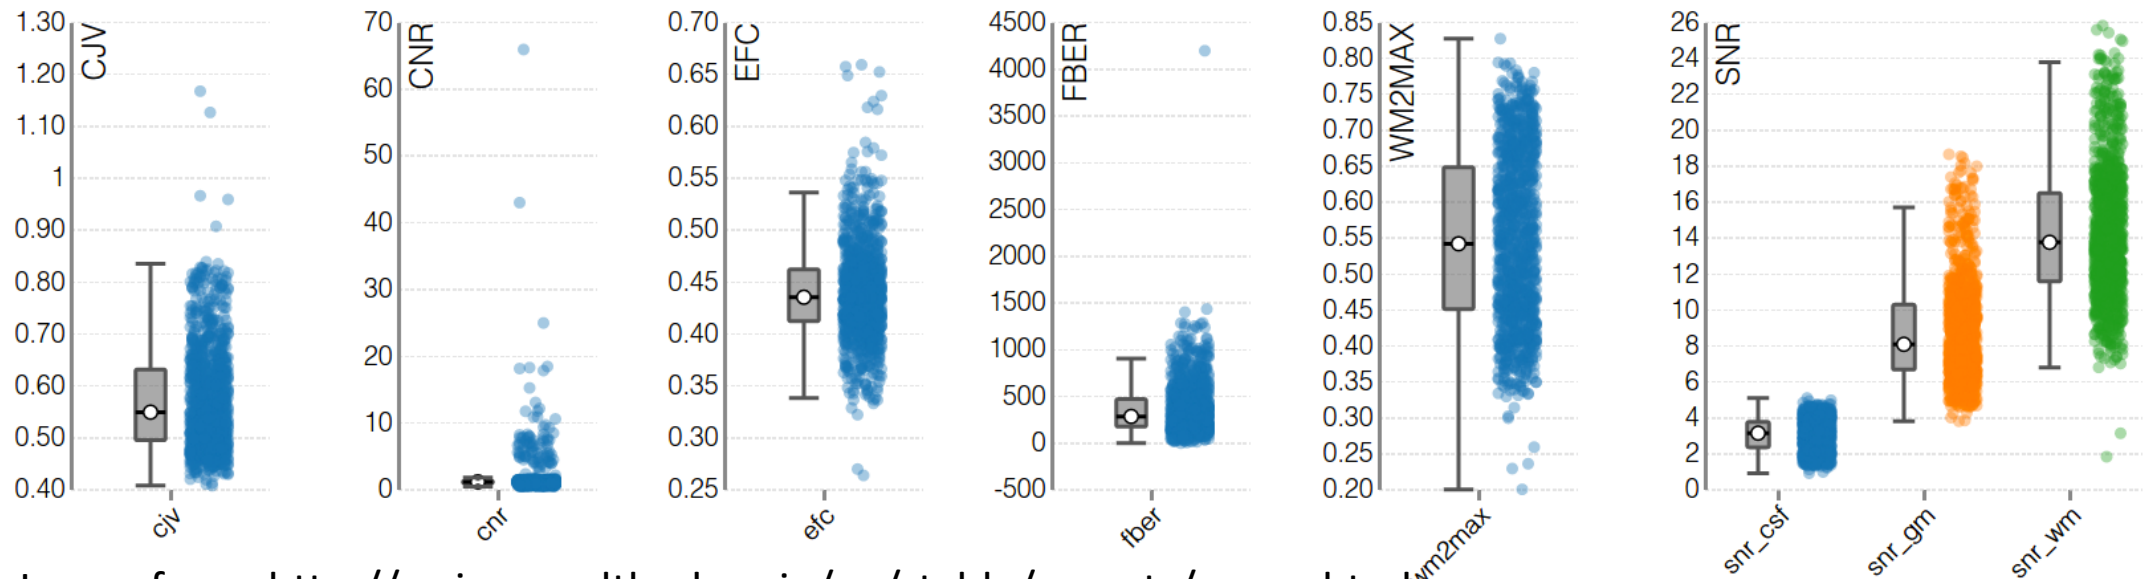


Image from: <http://mriqc.readthedocs.io/en/stable/reports/group.html>

MRIQC code: <https://github.com/poldracklab/mriqc>


MRIQC new web API: <https://mriqc.nimh.nih.gov/>

Real time observation of motion

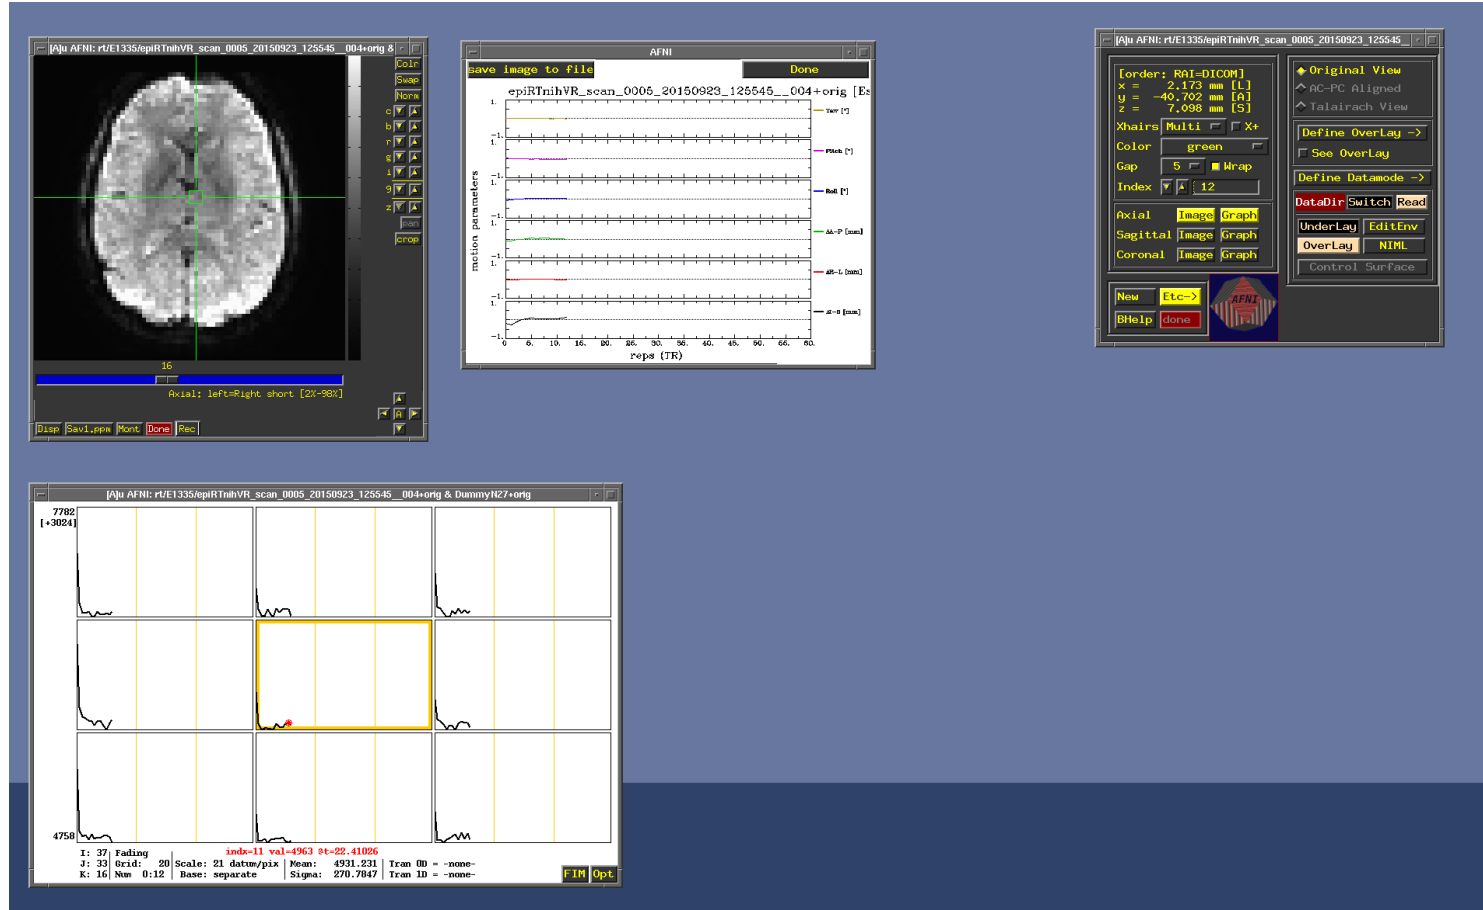


AFNI real time interface

Real time observation of motion

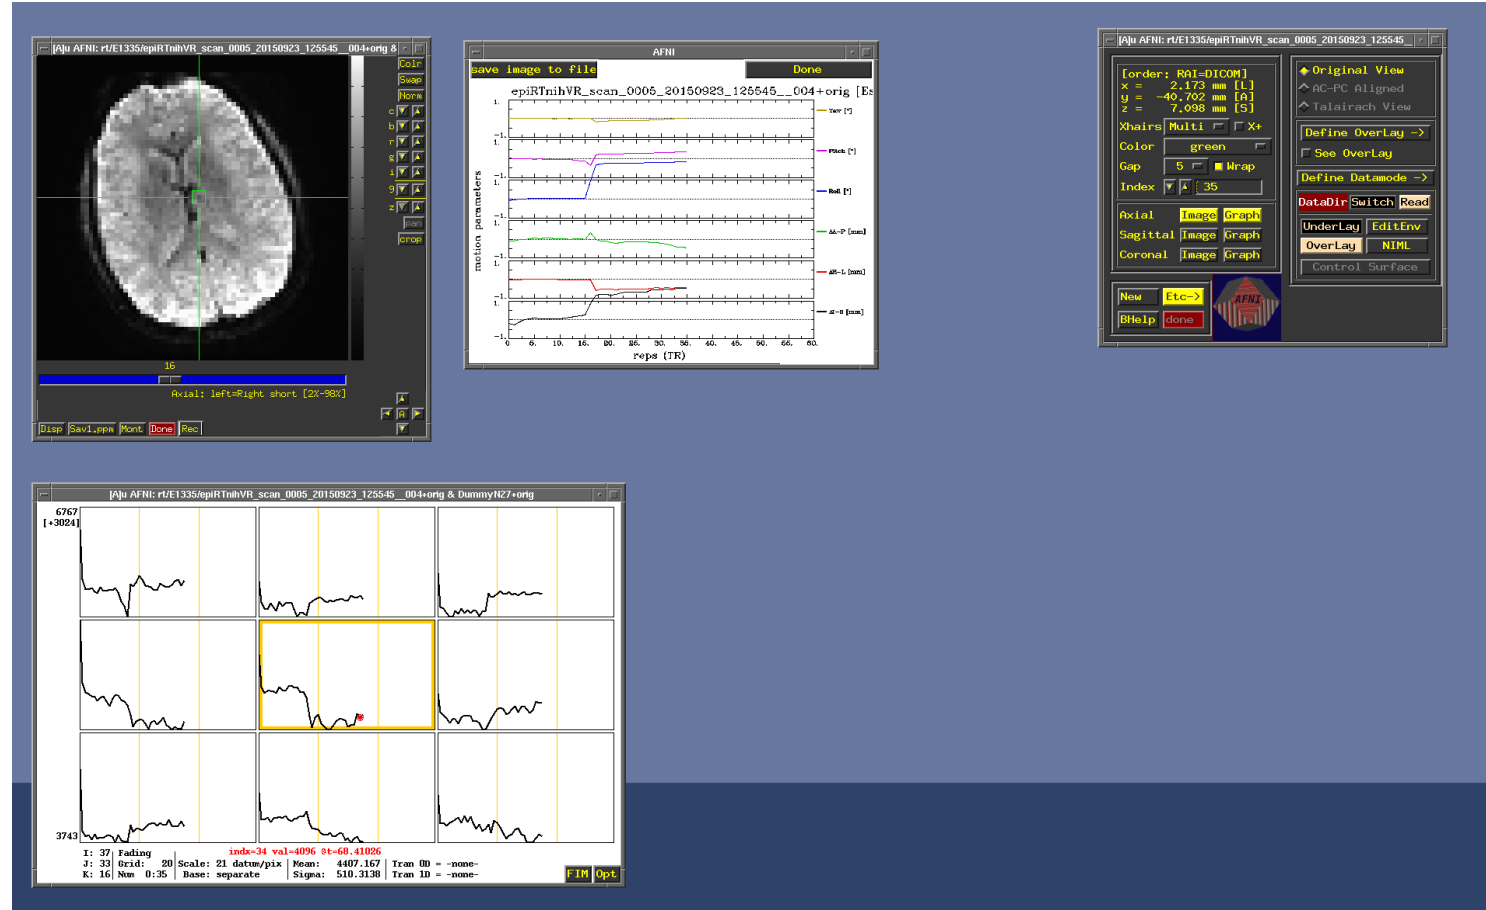

AFNI real time interface



Real time observation of motion

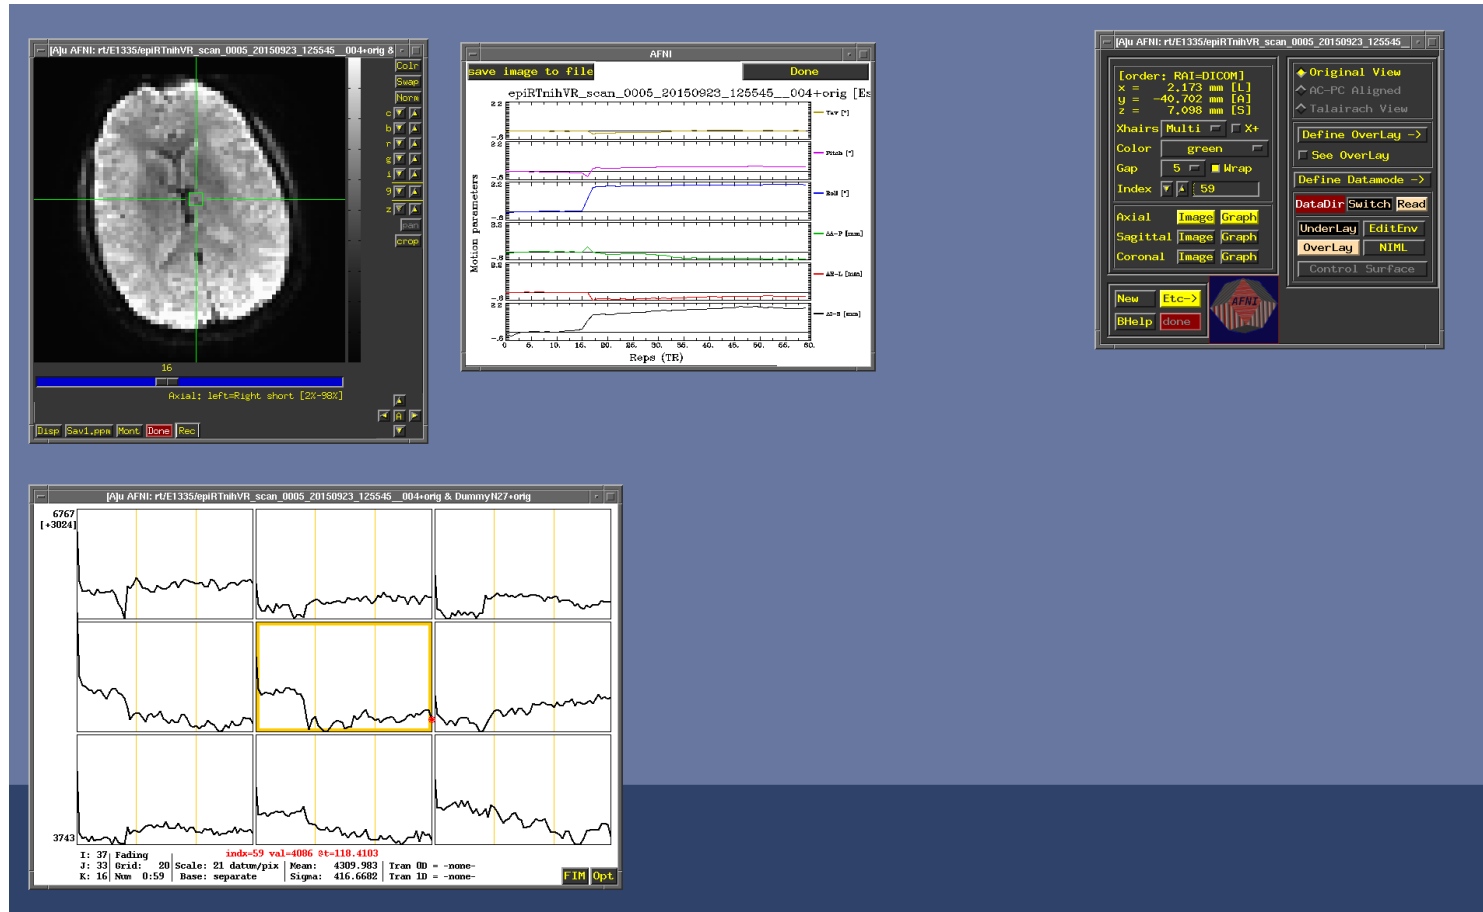

AFNI real time interface

Real time correlations as a monitoring tool

Respiration artifacts

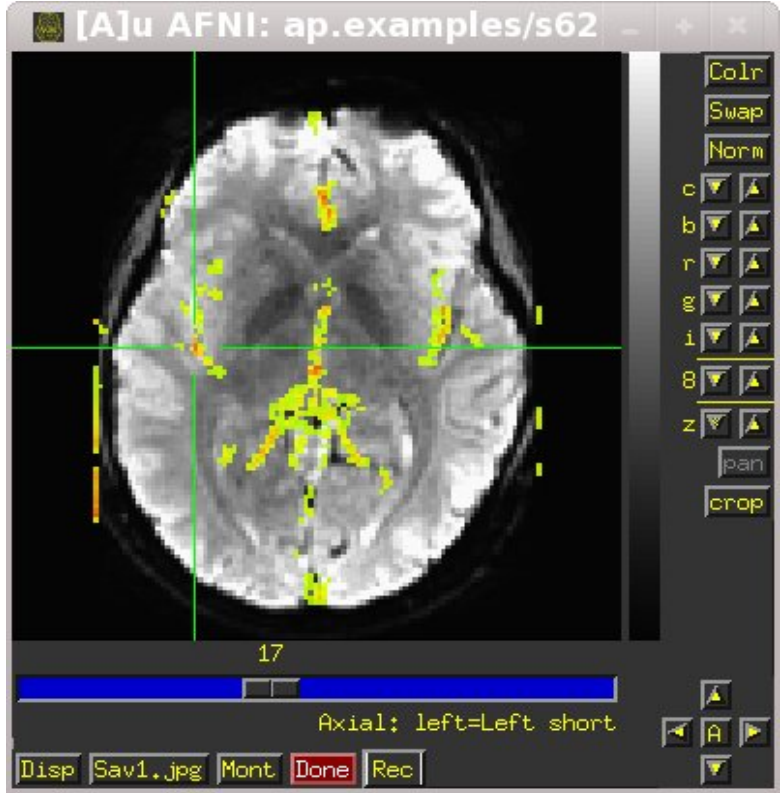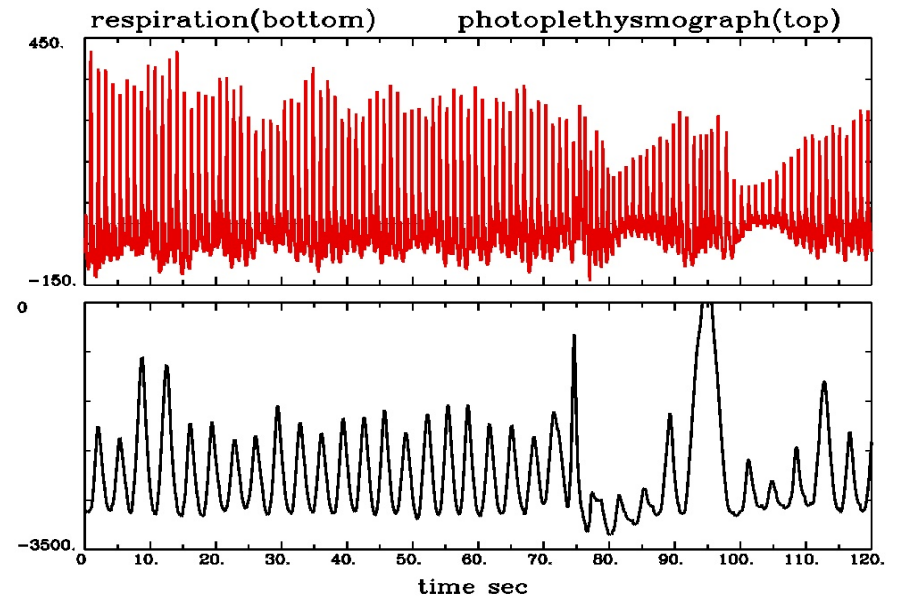

Using InstaCorr in AFNI

Correlations for artifact monitoring



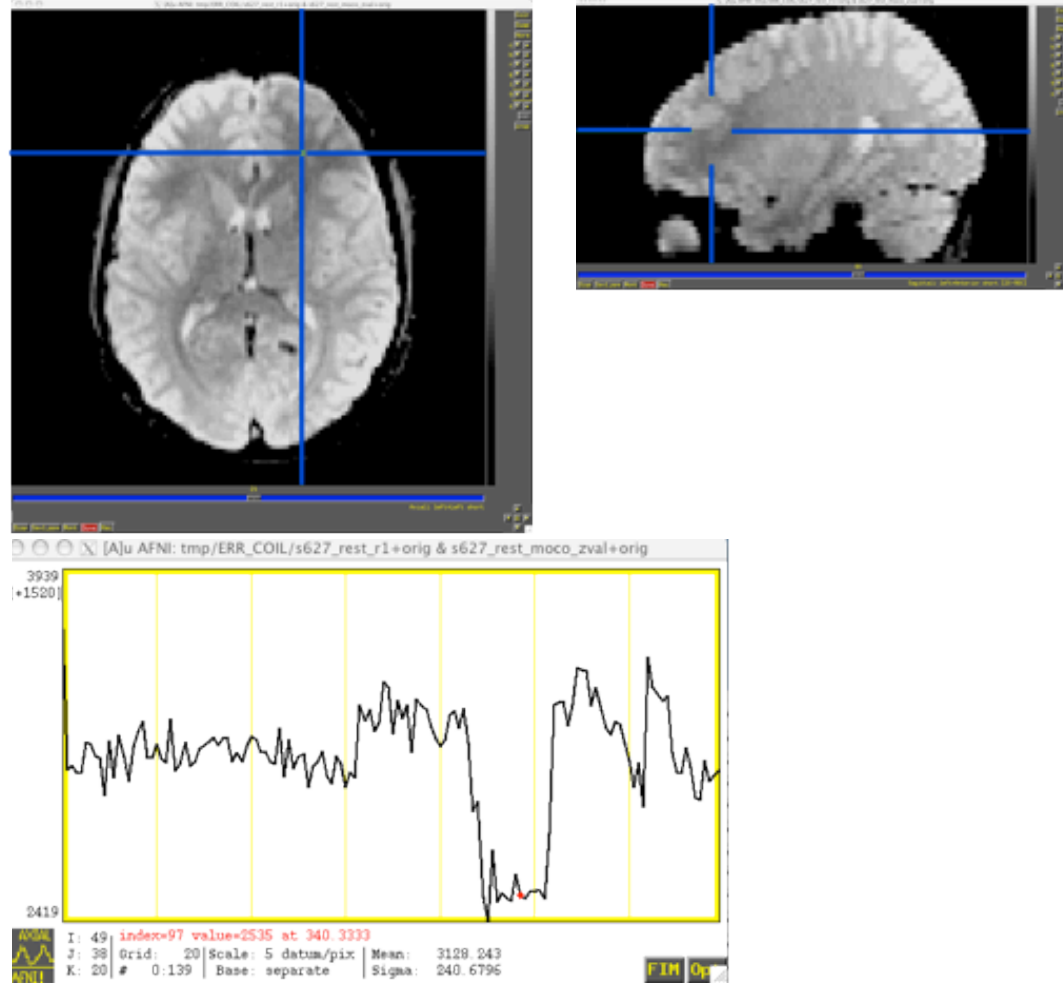


Image by Ziad Saad: https://afni.nimh.nih.gov/pub/dist/edu/latest/afni_handouts/BiasSources_RS-FMRI.pdf


Correlations for artifact monitoring

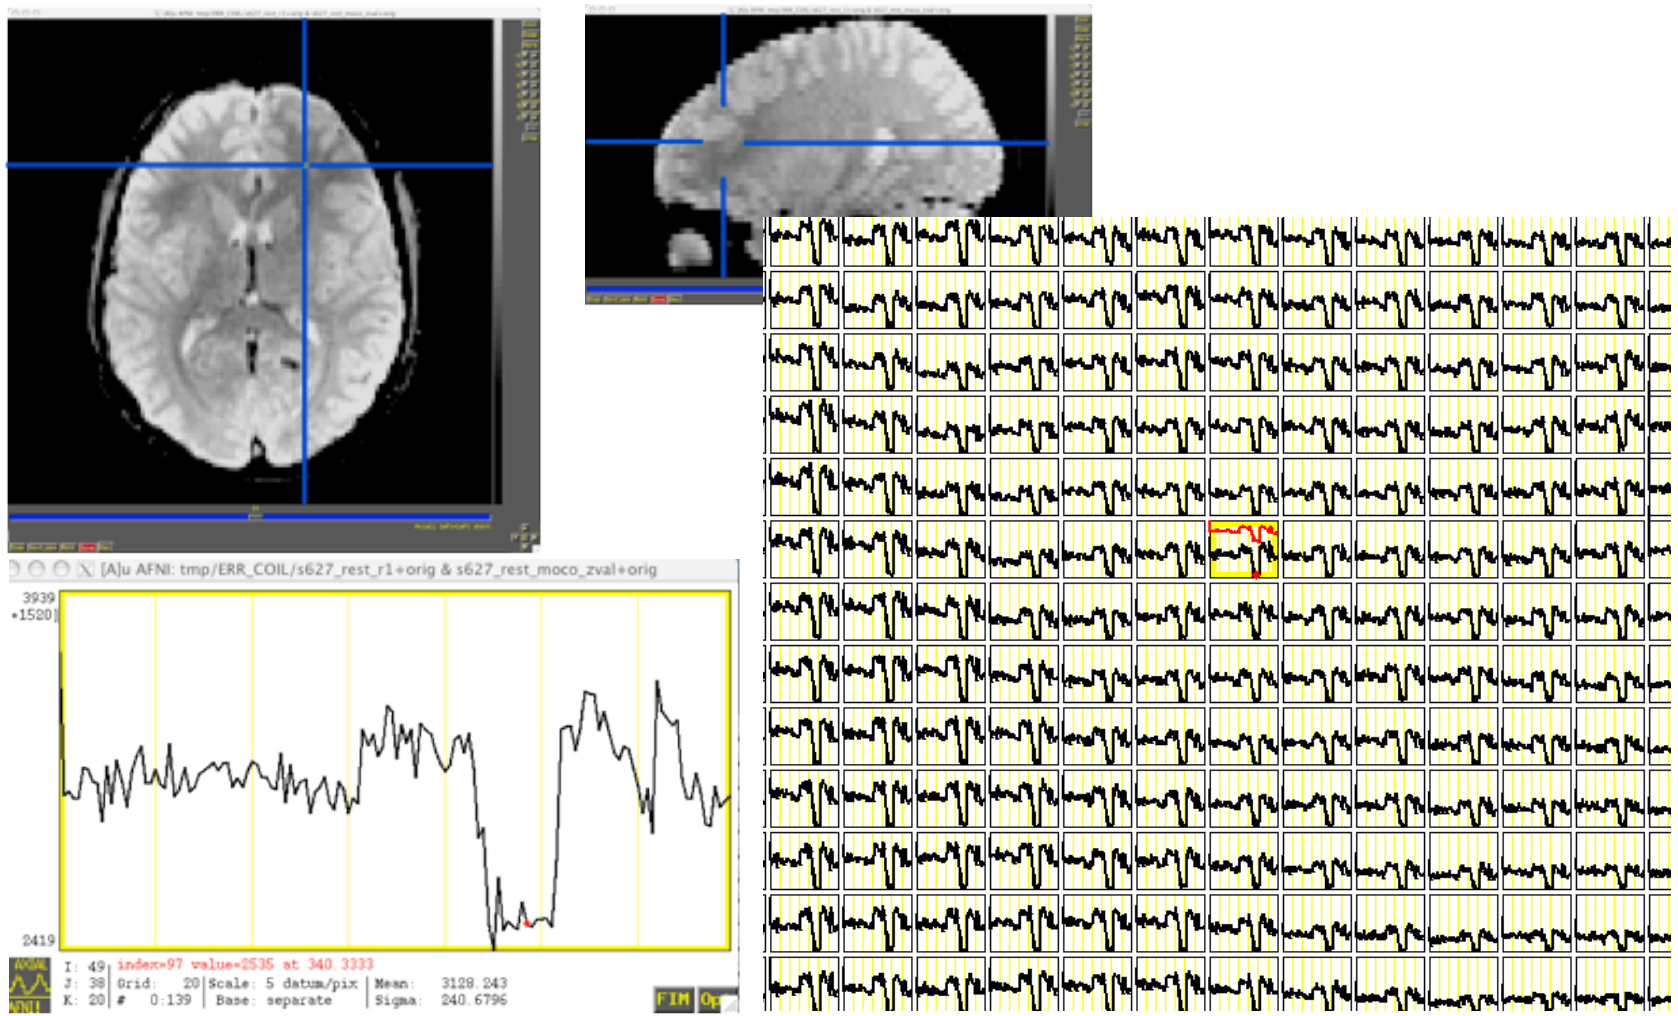

Correlation Map

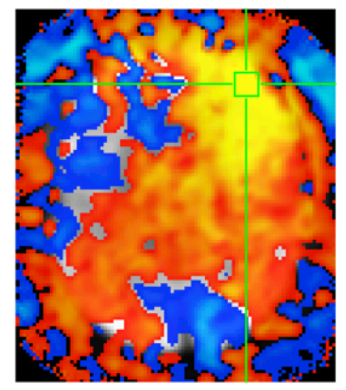

Eroded WM

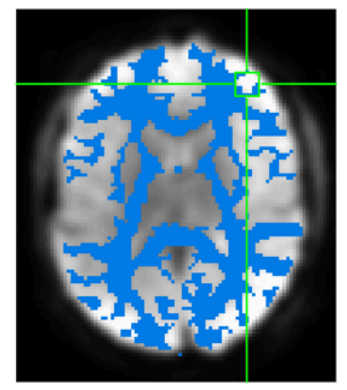

ρ
-1 -/+0 +1

Using AFNI InstaCorr

Summary

- Noise from many sources will always exist in fMRI data
- The more you understand noise sources and what acquisition decisions affect them, the better you can control for noise in acquisition and correct for noise in post-processing

Acknowledgements

Laurentius Huber

Ben Inglis

Vinai Roopchansingh

Bob Cox

Peter Bandettini