

Perfusion Imaging

Lalith Talagala, Ph.D.

NIH MRI Research Facility
National Institute for Neurological Disorders and Stroke
National Institutes of Health, Bethesda, MD

Perfusion Imaging: Outline

- Introduction
- Dynamic Susceptibility Contrast (DSC)
 - Method
 - Quantification
 - Examples
- Arterial Spin Labeling (ASL)
 - Method
 - Labeling Techniques
 - Quantification
 - Examples

Definitions

Perfusion – capillary blood flow delivered to tissue

MRI methods can assess

- blood flow – ml blood / min / 100 g of tissue
- blood volume – ml blood /100 g of tissue
- mean transit time – seconds


Normal values for brain

	Gray Matter	White Matter
CBF (ml /min/100 g)	60 - 80	20 - 30
CBV (ml / 100 g)	4 - 6	2 - 4
MTT (s)	4 - 5	5 - 6

Perfusion MRI


◆ Dynamic Susceptibility Contrast (DSC)

- Requires contrast injection
- Large signal changes, Fast
- Single application (clinical)

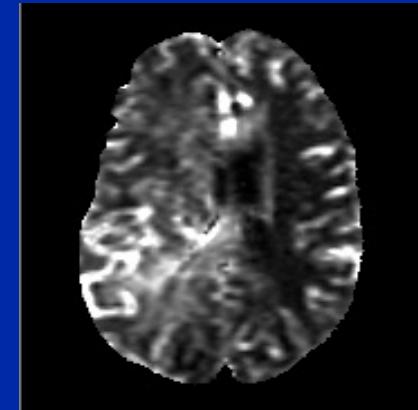


◆ Arterial Spin Labeling (ASL)

- No external contrast required
- Small signal change, Slow
- Multiple measurements (clinical and research)

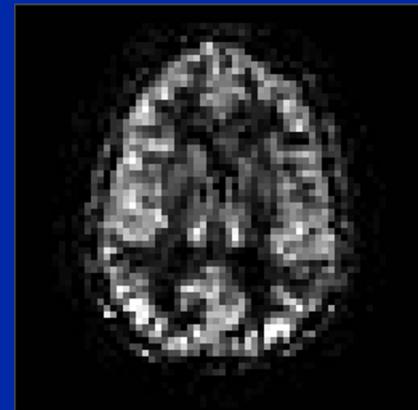

Dynamic Susceptibility Contrast (DSC)

Monitor passage of Gadolinium contrast through tissue using rapid T2*/T2 weighted MRI

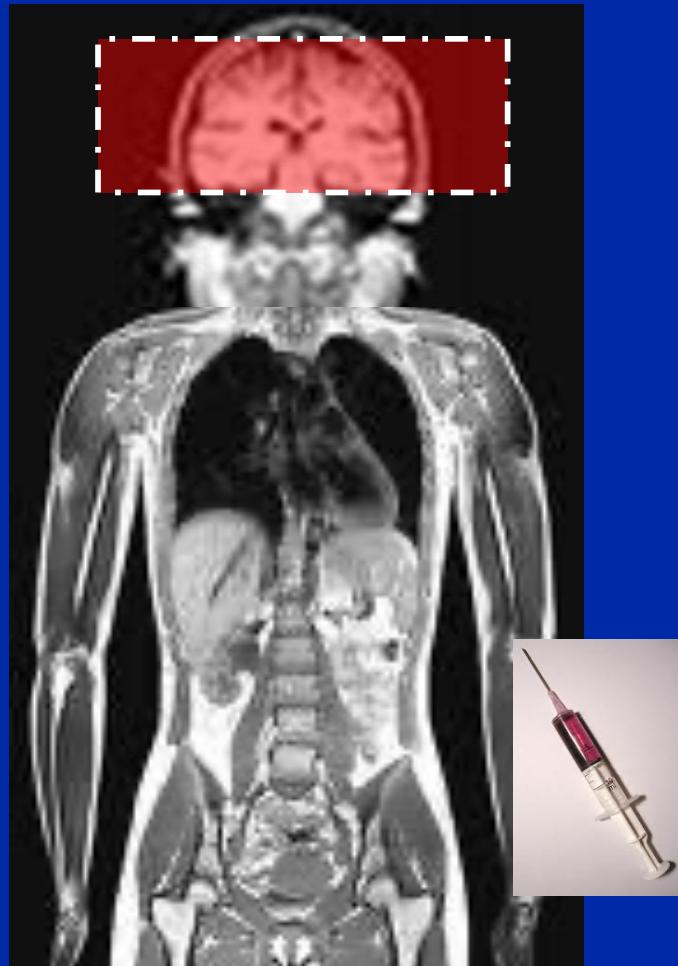

Imaging

Gradient Echo EPI

TR ~1.5- 2 s

TE = 30 -50 ms


~1.5 min

Bolus Injection

Gd 0.1 - 0.2 mmol/kg

DSC - Mechanism

Gd Chelates: Paramagnetic, Intravascular

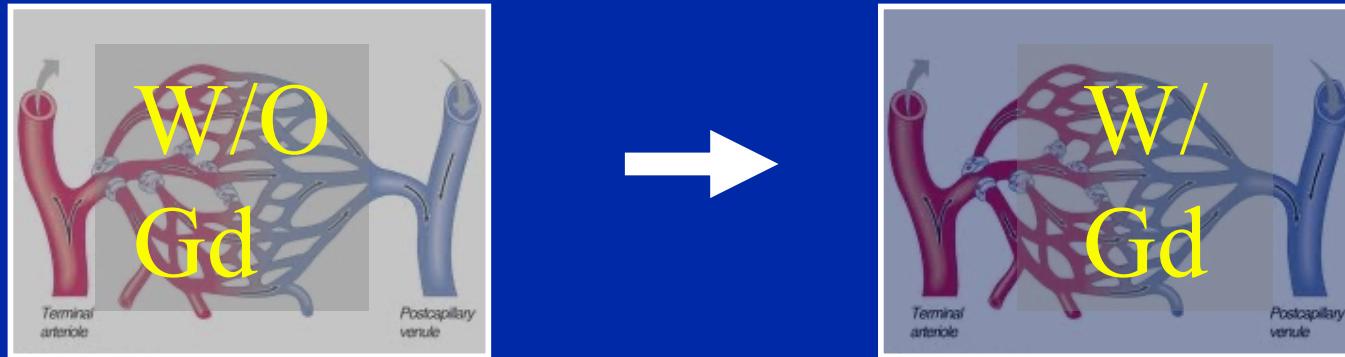

Tissue/ Blood $\Delta\chi$


Field Inhomogeneity

R_2^* ($-1/T_2^*$)

GE/SE MRI Signal




DSC – Passage of Gd through tissue

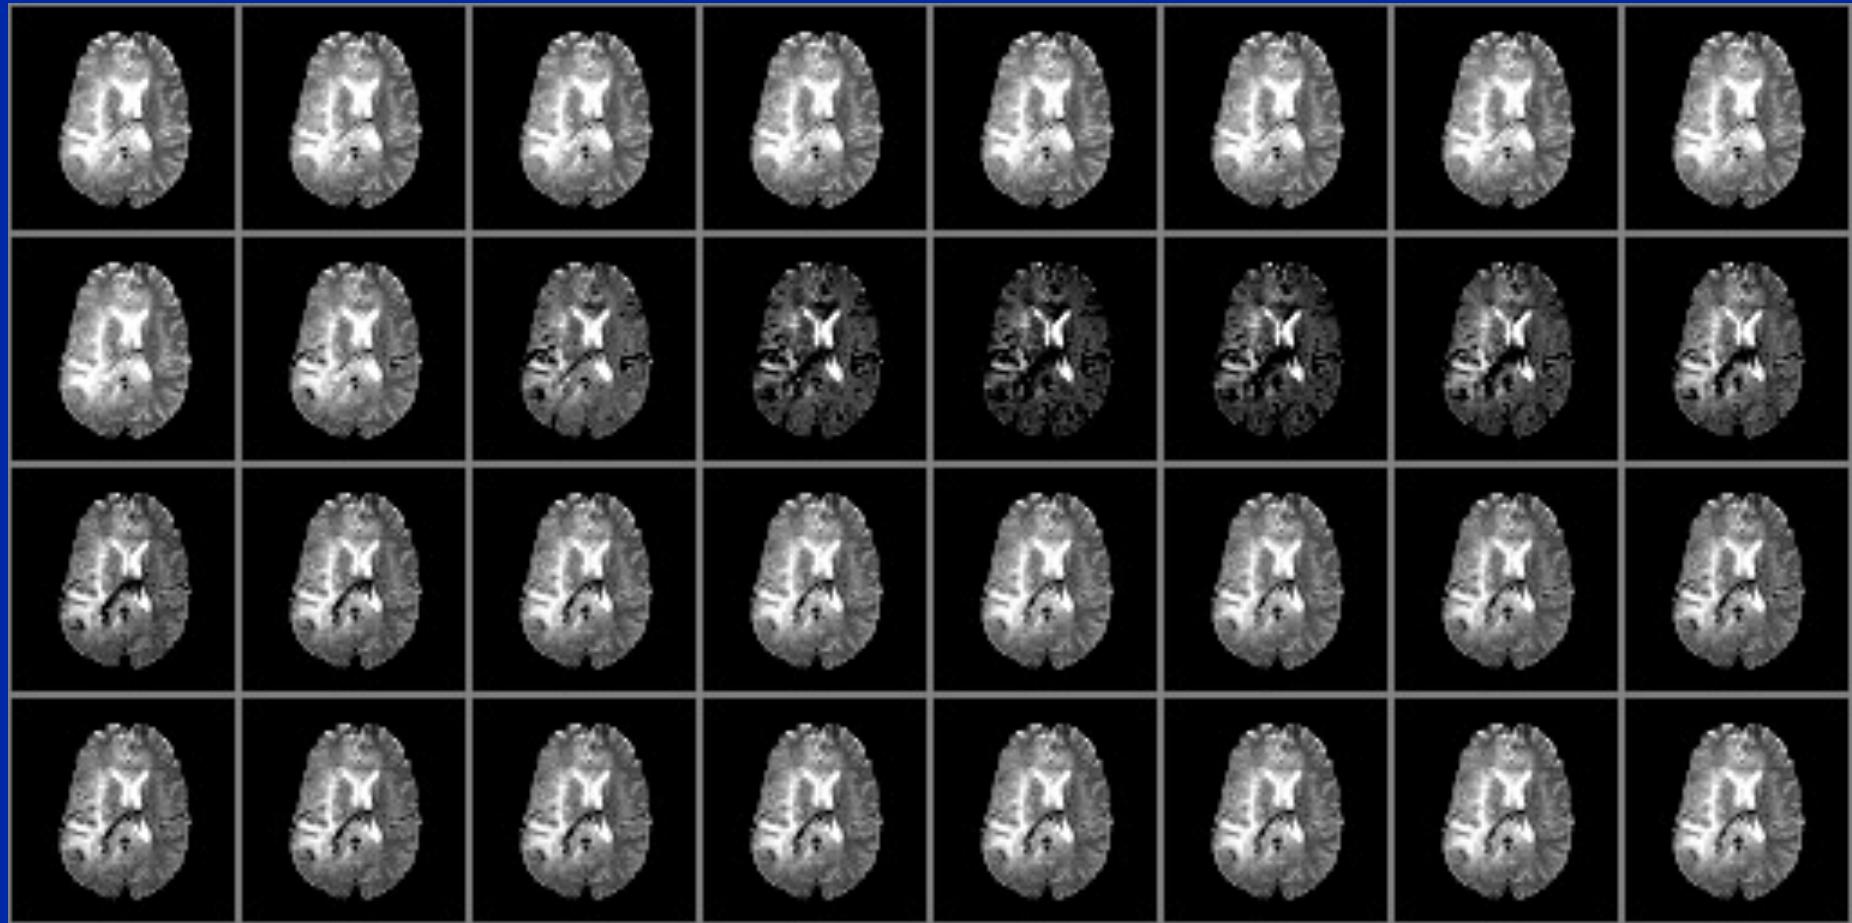

1.5 T, 0.1 mmol/kg, GE- EPI, TE = 50 ms, TR = 2 s

DSC – Signal vs Time

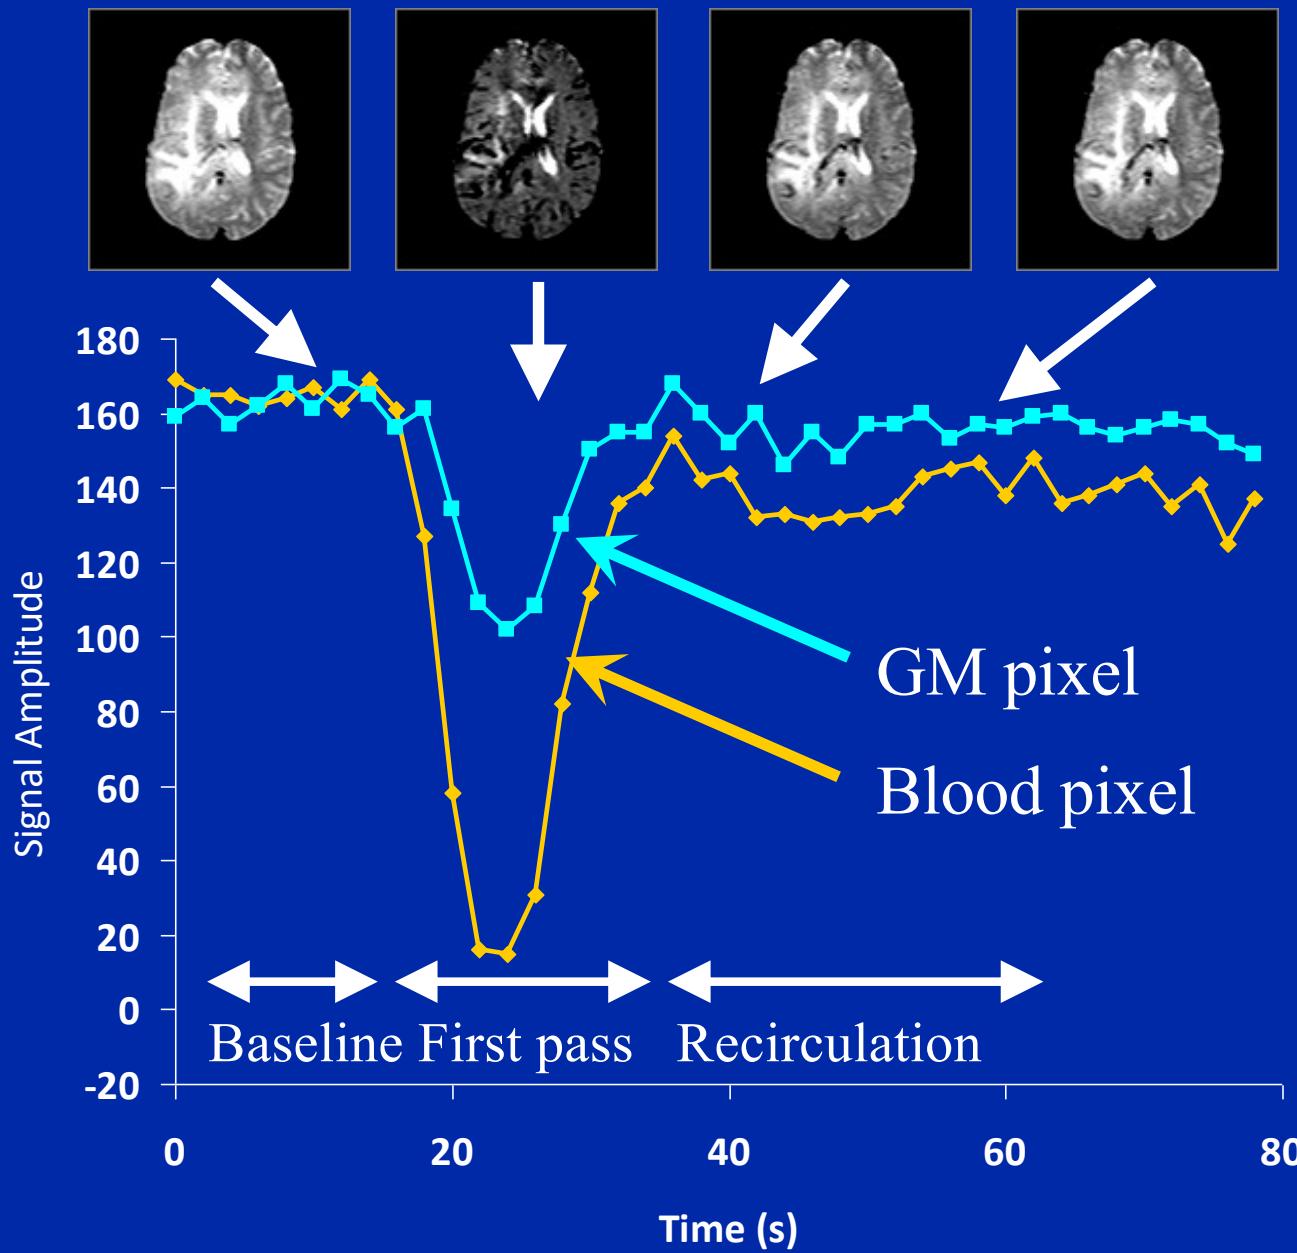

DSC: Signal loss to Concentration

$$\Delta R_2^* = k \cdot C \quad \left. \right\} \quad S_c = S_0 \cdot \exp(-TE \cdot \Delta R_2^*) \quad \boxed{\quad}$$

k – proportionality constant


C – Gd concentration

S_c – Signal with Gd


S_0 – Baseline signal without Gd

$$C = -\frac{1}{k \cdot TE} \ln \frac{S_c}{S_0}$$

DSC: Concentration vs time

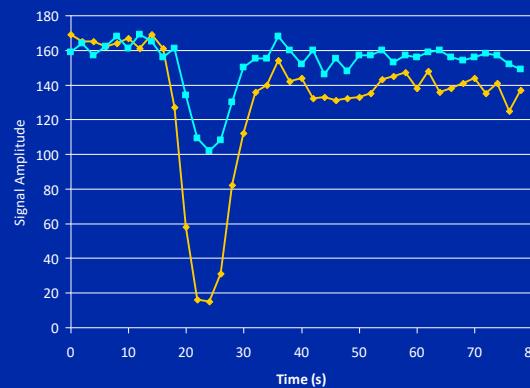

$$\text{C} = -\frac{1}{k \cdot TE} \ln \frac{S_c}{S_0}$$


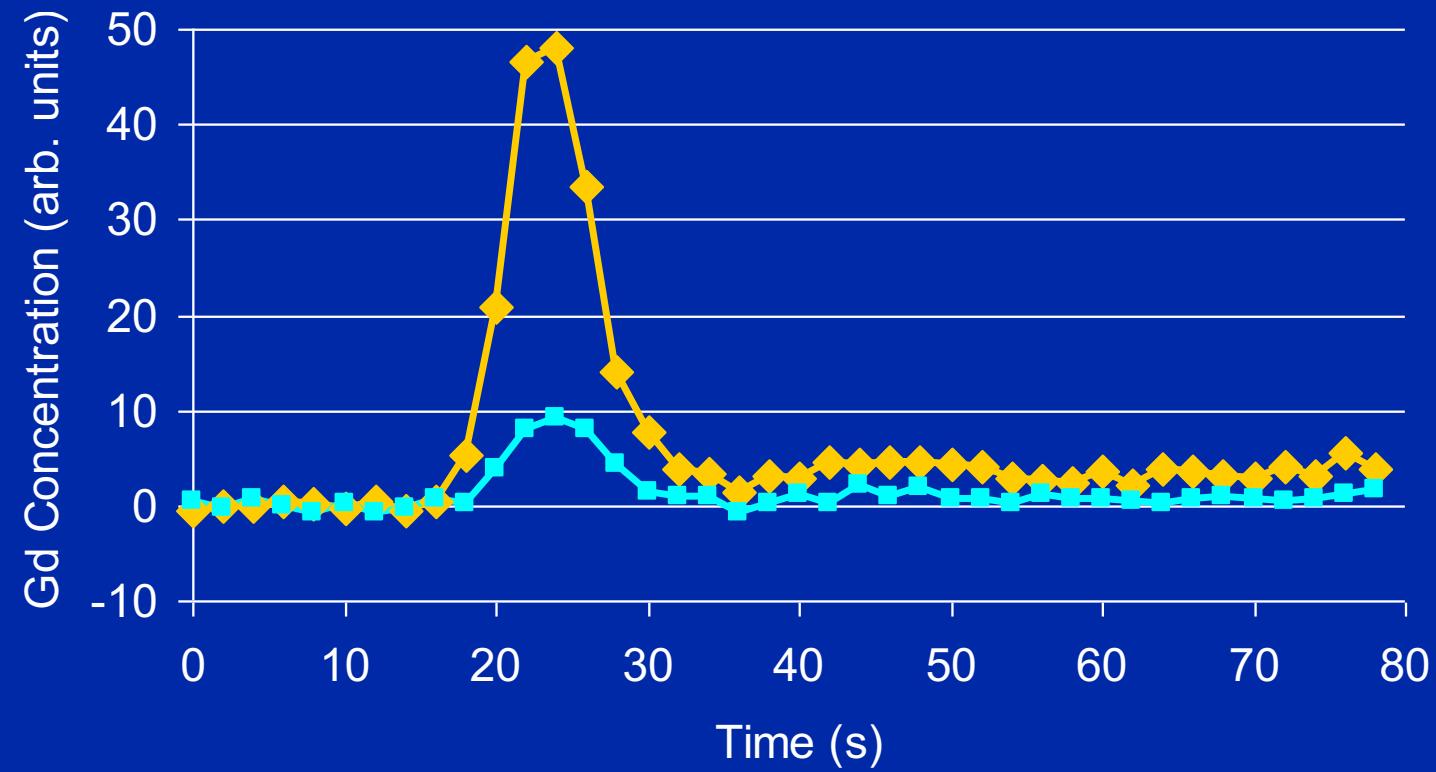


DSC – CBV, CBF, MTT ?

F (ml/min)


$C_{art}(t)$

Arterial
input
function
(AIF)

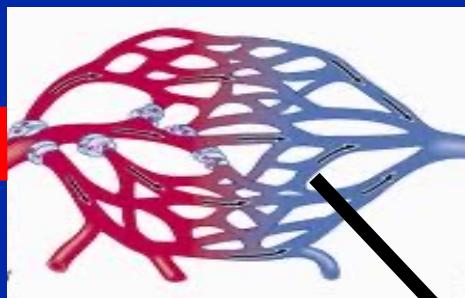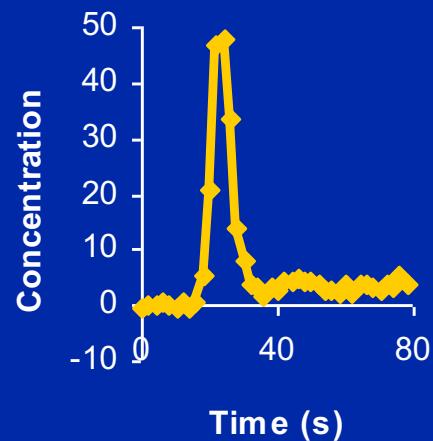

$C_{tis}(t)$

Tissue
Response

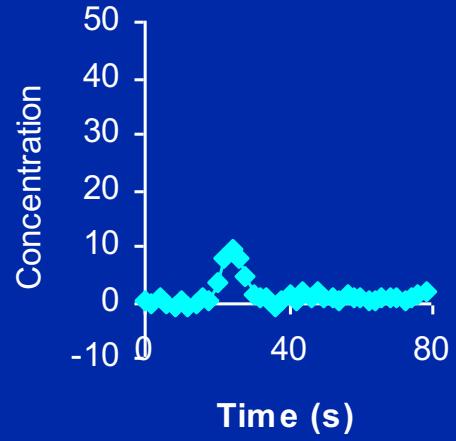


Tracer
Kinetic
Theory

$$MTT = \frac{CBV}{CBF}$$

DSC- Calculation of CBV

$$C_{art}(t) \xrightarrow{F} C_{tis}(t) \xrightarrow{} C_{vein}(t)$$

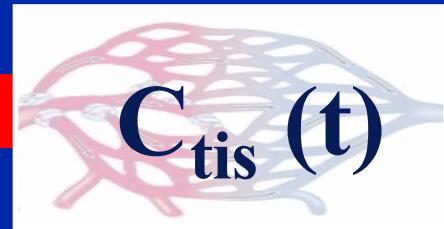


$$CBV = \frac{k_H}{\rho} \frac{\int C_{tis}(t) \cdot dt}{\int C_{art}(t) \cdot dt} \rightarrow \frac{\text{Baseline}}{\text{Peak}}$$

The diagram illustrates the calculation of CBV using the formula above. It shows a baseline signal with a small peak (blue) and a signal with a large peak (yellow), with the area under each peak shaded. A horizontal line with arrows at both ends connects the two signals, representing the ratio of the areas.


DSC- Calculation of CBF and MTT

$$C_{art}(t) \xrightarrow{F} C_{tis}(t) \xrightarrow{} C_{vein}(t)$$

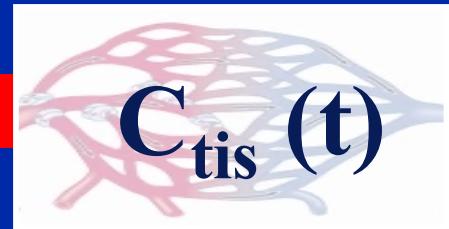

$$\check{C}_{tis}(t) = CBF \cdot \int_0^t C_{art}(\tau) R(t - \tau) d\tau$$


$$R_{scl}(t) = Deconvol(C_{tis}(t), C_{art}(t))$$

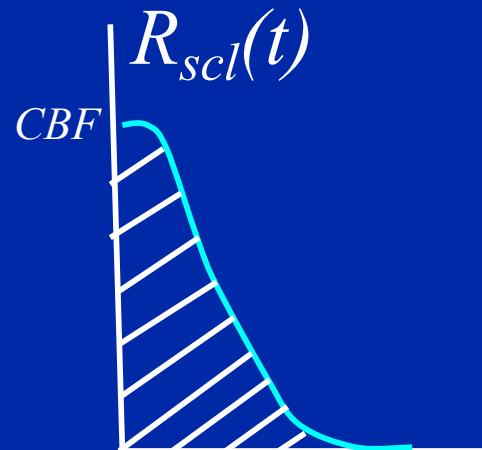


$$CBF = R_{scl}(0)$$

$$MTT = \frac{CBV}{CBF} \text{ and } \frac{\int R_{scl}(t) \cdot dt}{R_{scl}(0)}$$


DSC – CBV, CBF, MTT maps

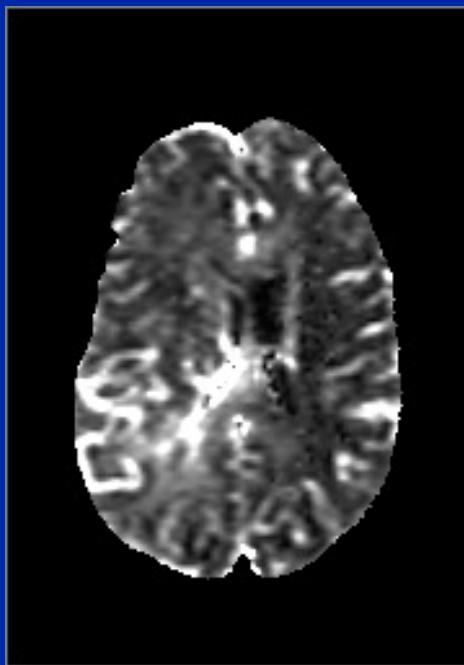

CBV

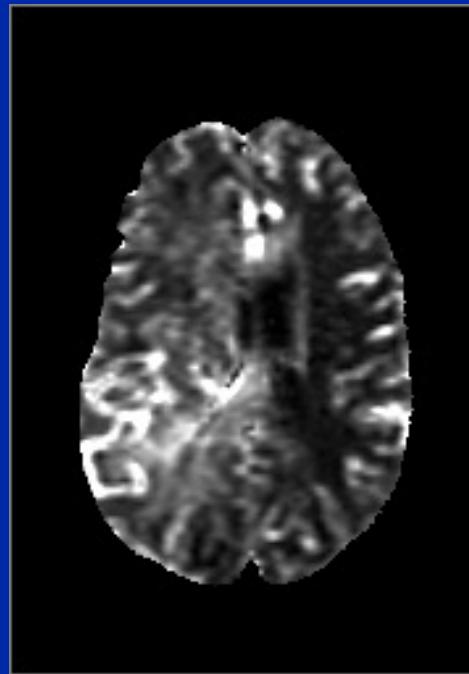


CBF

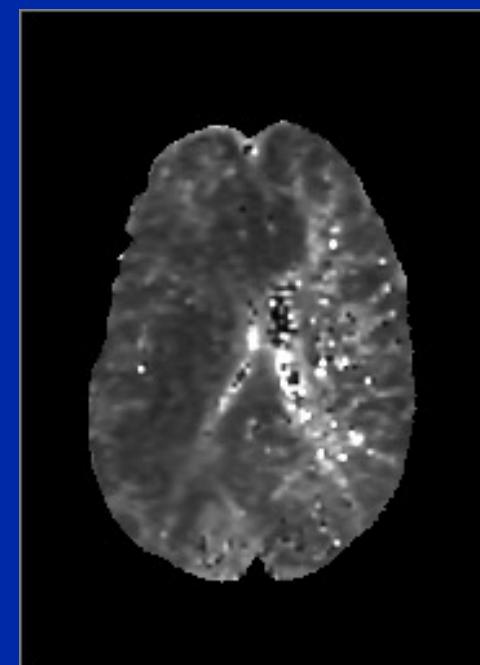


MTT

DSC – CBV, CBF, MTT maps

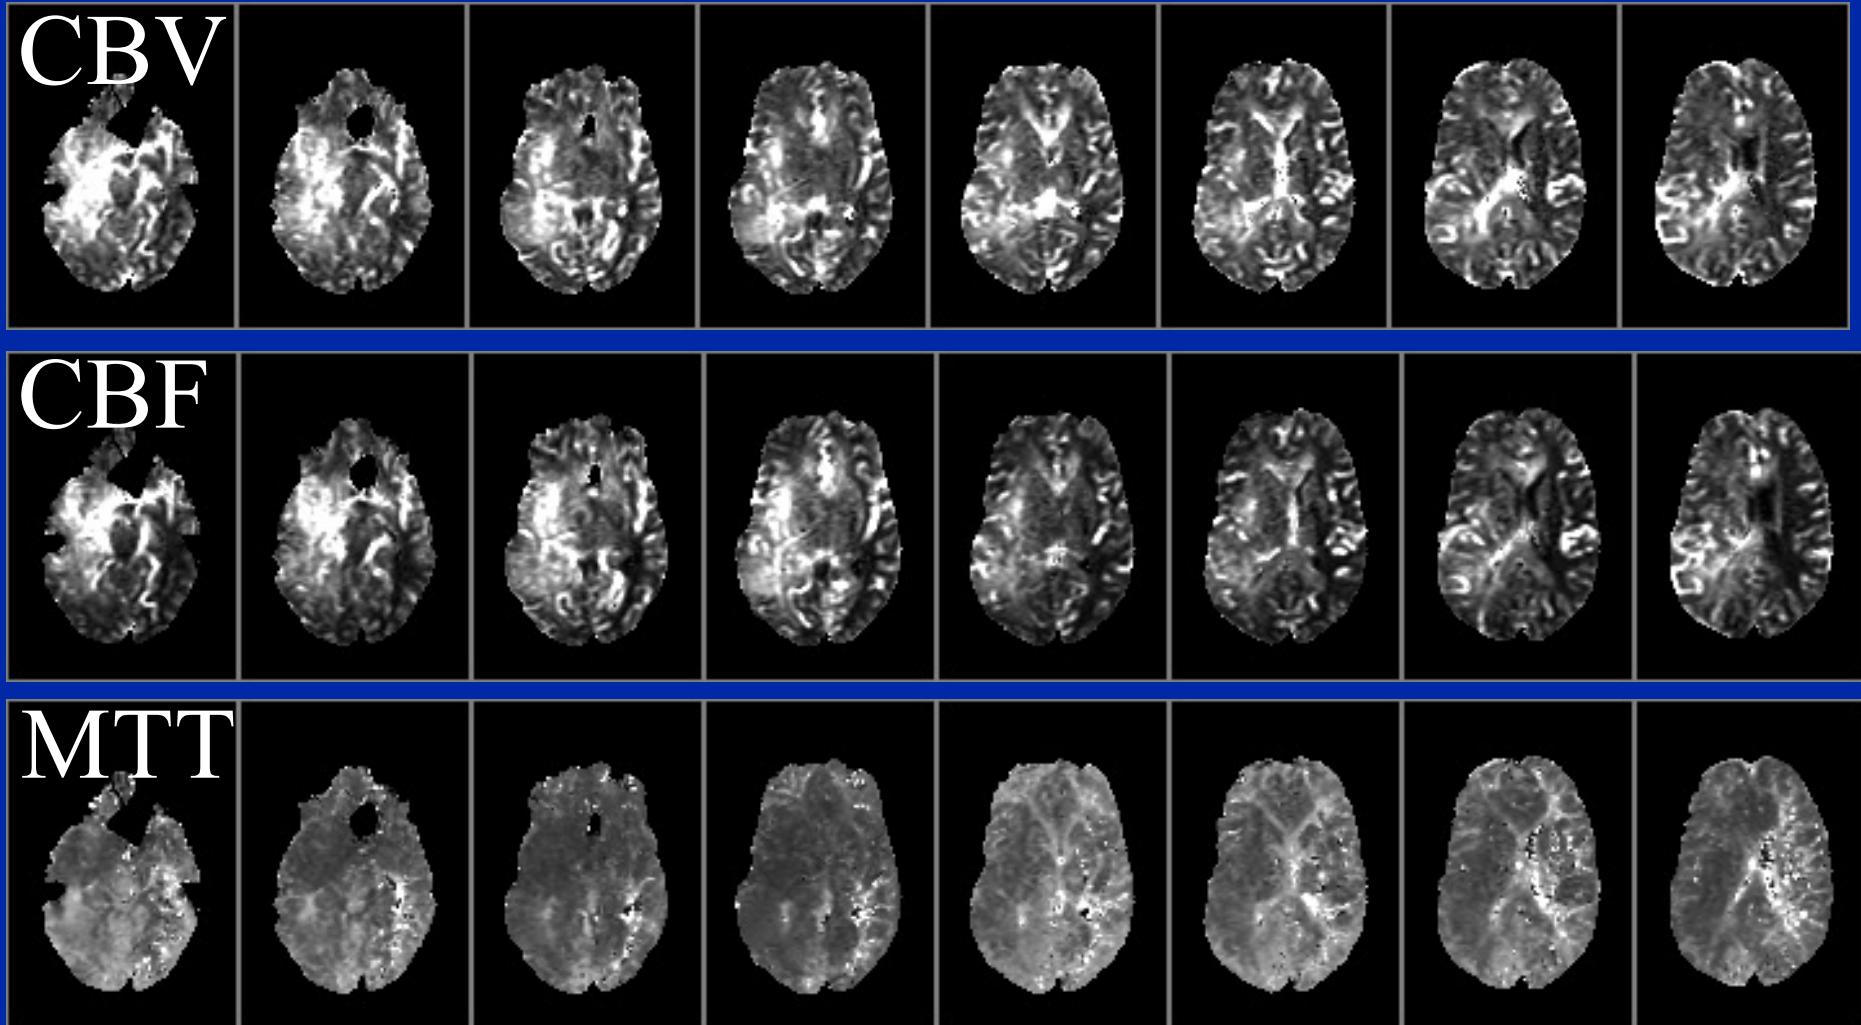

DSC – CBF maps

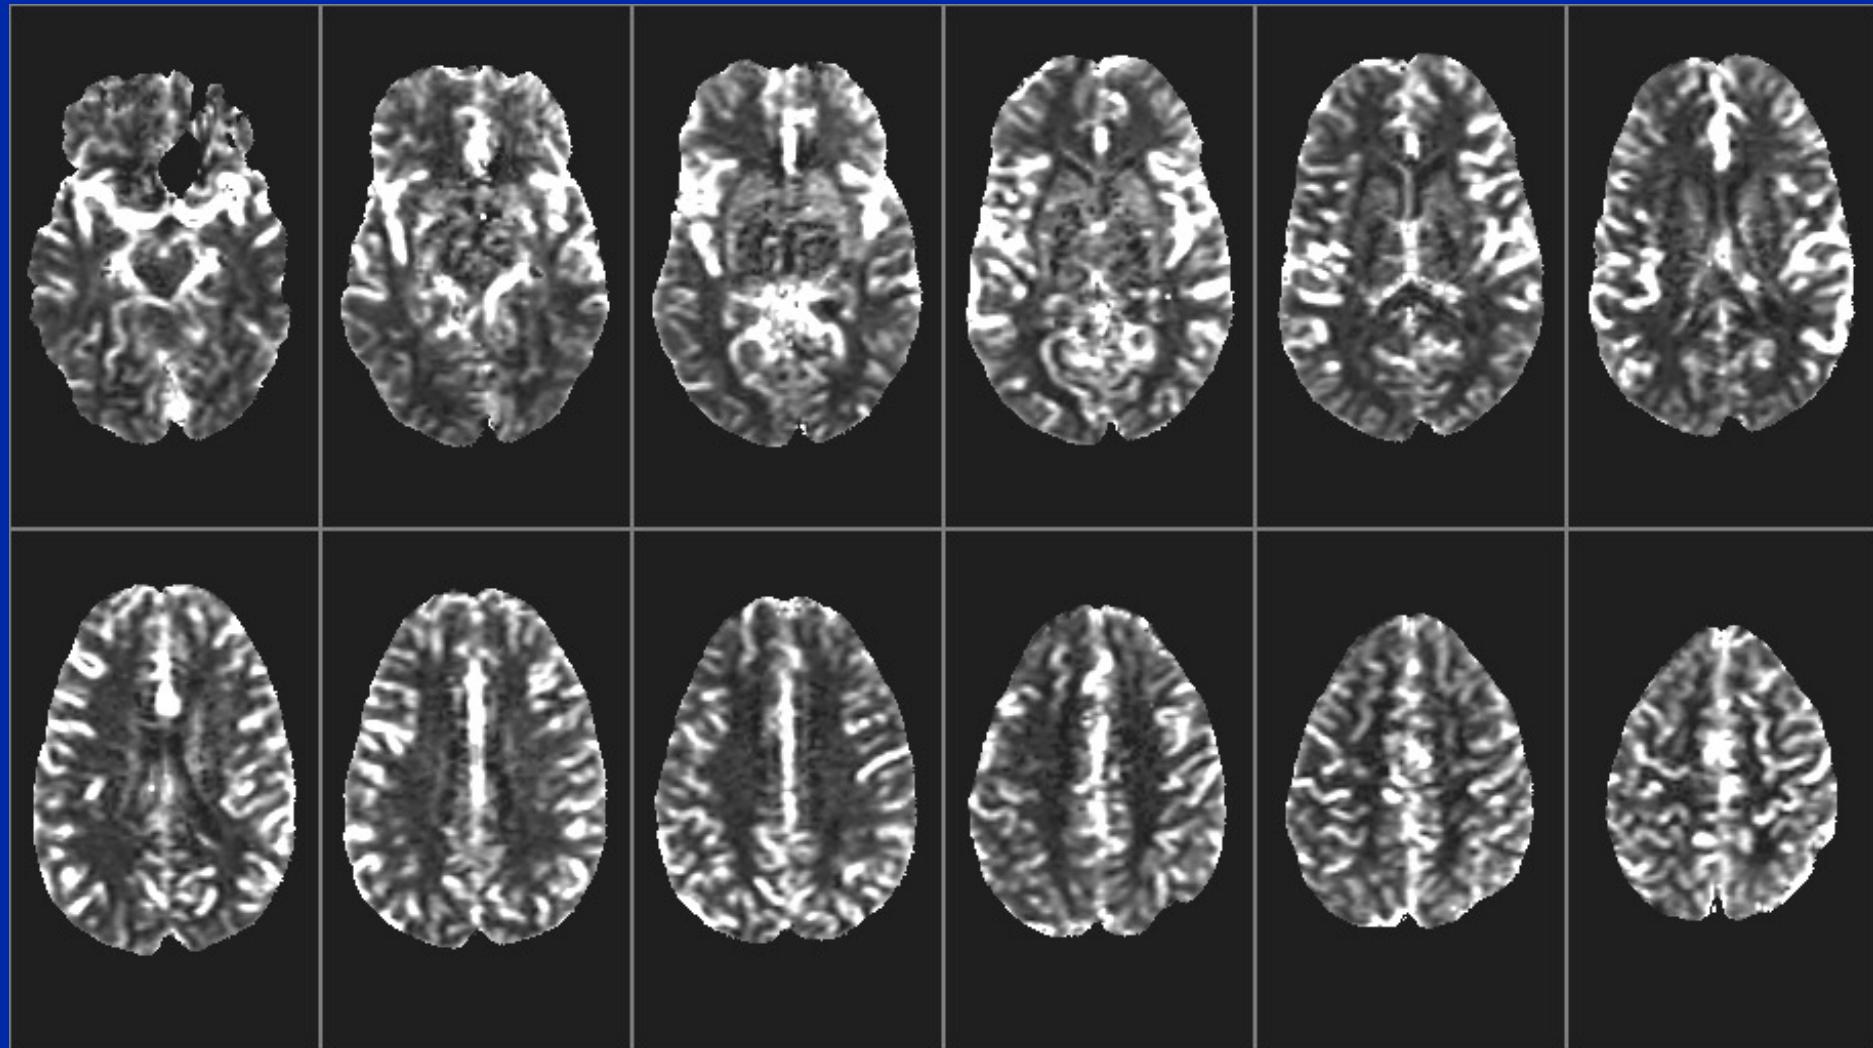


1.5 T, 0.1 mmol/kg, GE- EPI, TE = 50 ms, TR = 2 s

DSC: Quantification Issues


- Accuracy of $\Delta R_2^* \Leftrightarrow C$ relationship
 - Arteries (quadratic) and tissue (linear)
- Arterial input function (AIF) determination
 - Partial volume , vessel orientation effects
 - Truncation of the peak
 - Dispersion between measurement site and tissue (local AIF)
- Deconvolution errors
 - Sensitivity to noise
 - Sensitivity to bolus arrival times
- ◆ Absolute CBF/CBV require use of scaling factors determined separately

Arterial Spin Labeling (ASL)

Measure the change in MRI signal due to magnetic labeling (tagging) of inflowing blood

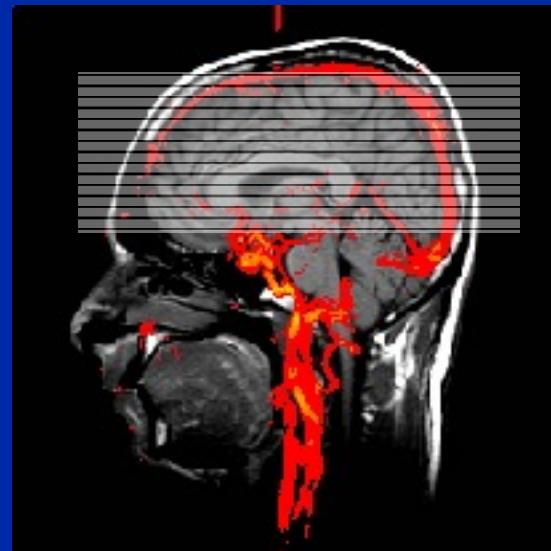

Control

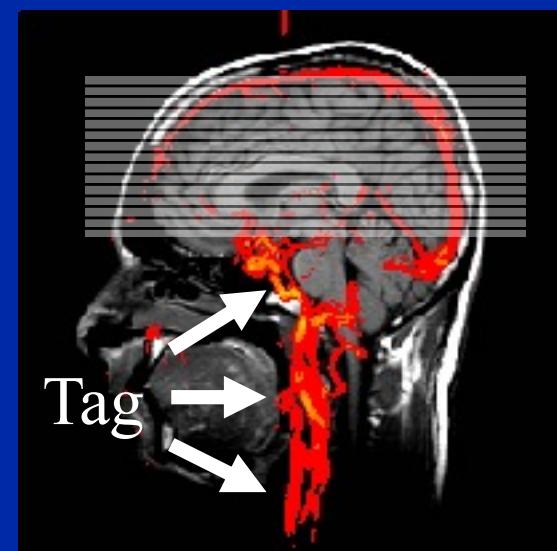

Label

=> Perfusion
Maps

LABELING


0.5 – 2.5 s

IMAGING

0.5 - 2 s 0.75 s

GE/SE EPI
TR ~ 2 - 5 s
TE = minimum
~ 4-5 minutes

ASL: Control/Label/Difference

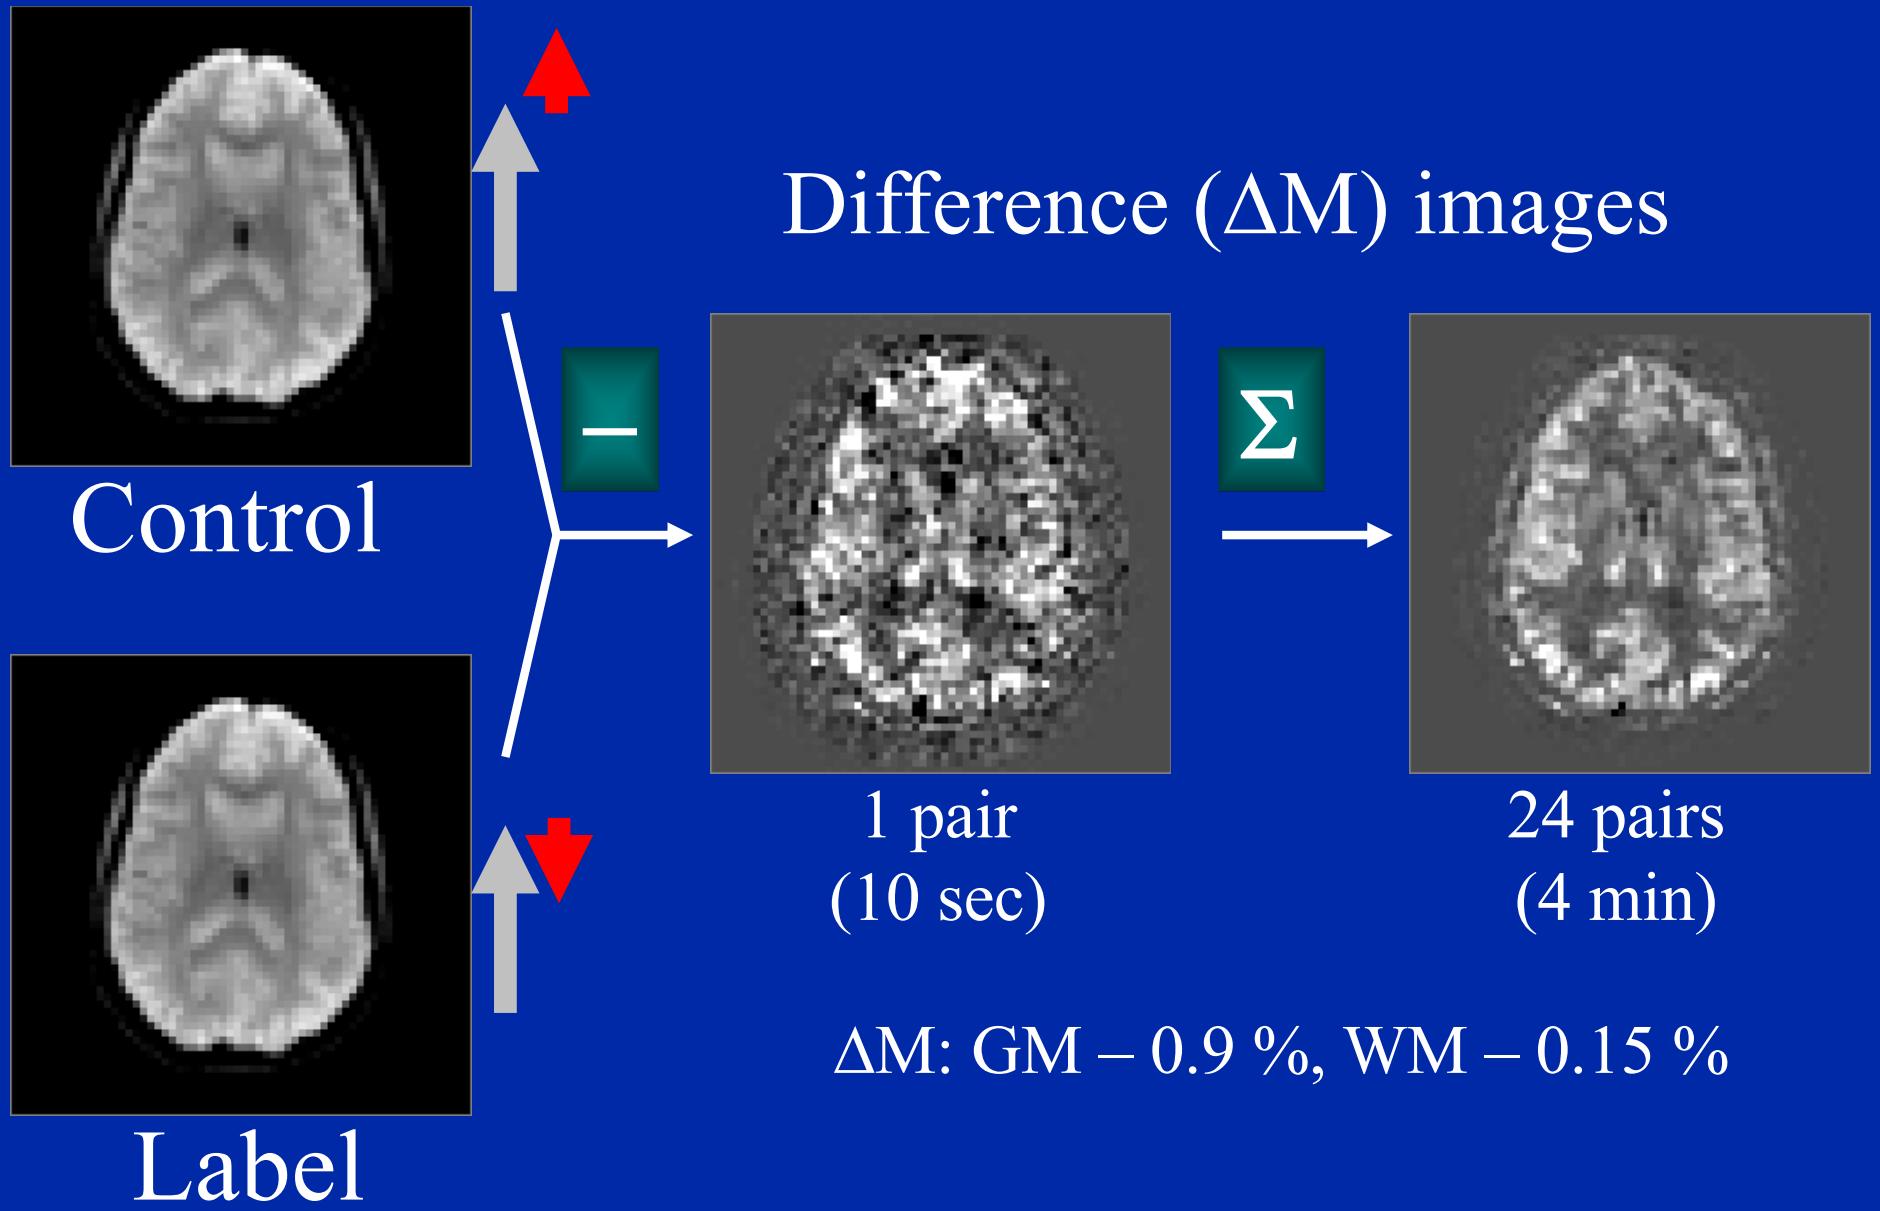


ASL: Labeling Strategies

◆ Pulsed ASL (PASL)

- ◆ Wide labeling slab
- ◆ Created by a short pulse (milliseconds)
- ◆ Input function – decaying exponential


(T1 of blood)

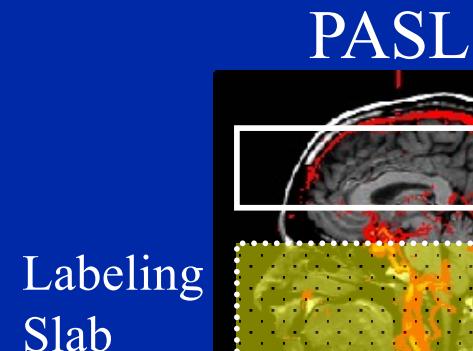

Labeling
Slab

◆ Continuous ASL (CASL)

- ◆ Narrow labeling plane
- ◆ Long duration (seconds)
- ◆ Input function – constant

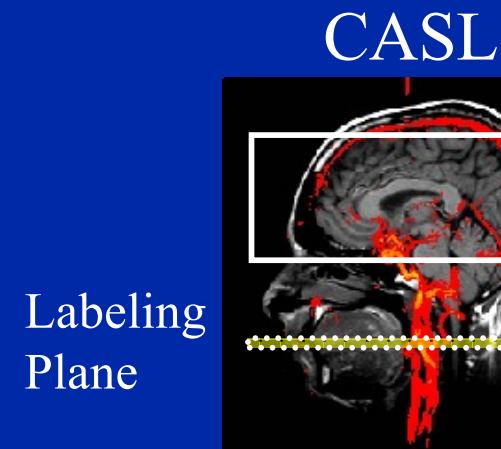

Labeling
Plane

ASL- Quantification of CBF

One compartment model: Labeled blood stays in the vasculature

PASL

$$CBF_{PASL} = \frac{\lambda}{2\alpha_0} \cdot \frac{\exp(w \cdot R_{1a})}{\tau \cdot \exp(-\tau \cdot R_{1a})} \cdot \frac{\Delta S}{S^{eqm}}$$

CASL

$$CBF_{CASL} = \frac{\lambda R_{1a}}{2\alpha_0} \cdot \frac{\exp(w \cdot R_{1a})}{[1 - \exp(-\tau \cdot R_{1a})]} \cdot \frac{\Delta S}{S^{eqm}}$$

R_{1a} – relaxation rate of arterial blood


α_0 – labeling efficiency

τ – labeling time

w – post labeling delay


λ – brain/blood partition coefficient of water

ASL: Pulsed Labeling (QUIPSS II)

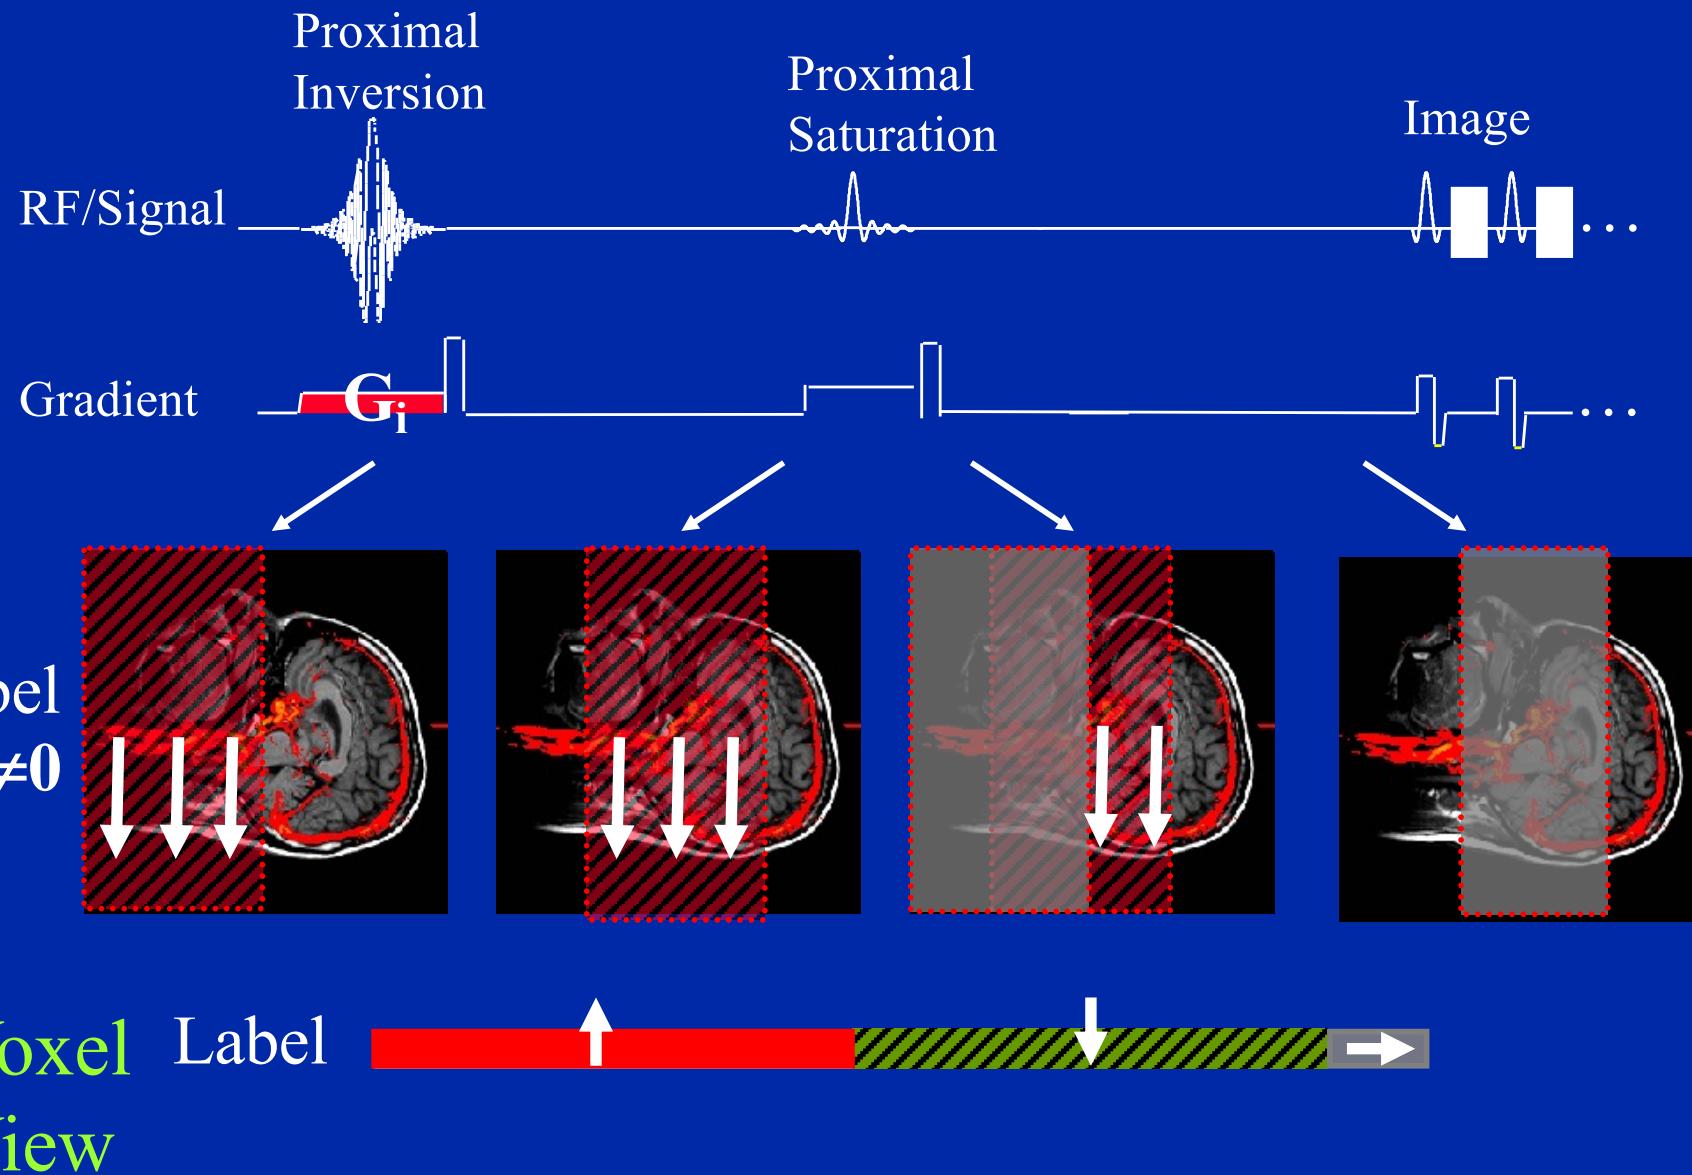


ASL: Pulsed Labeling (QUIPSS II)

Label
 $G_i \neq 0$

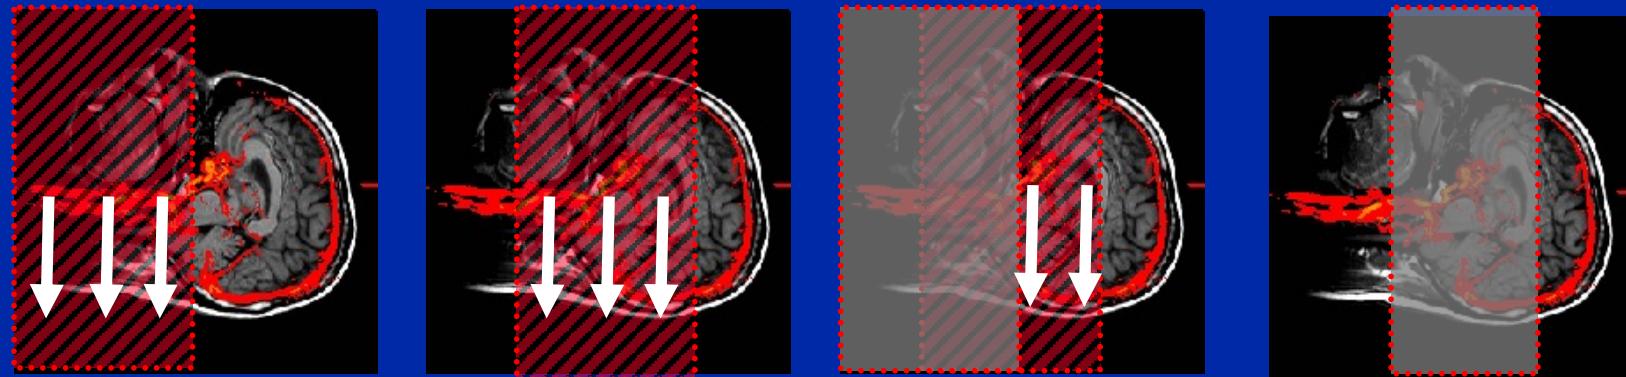

Control
 $G_i = 0$

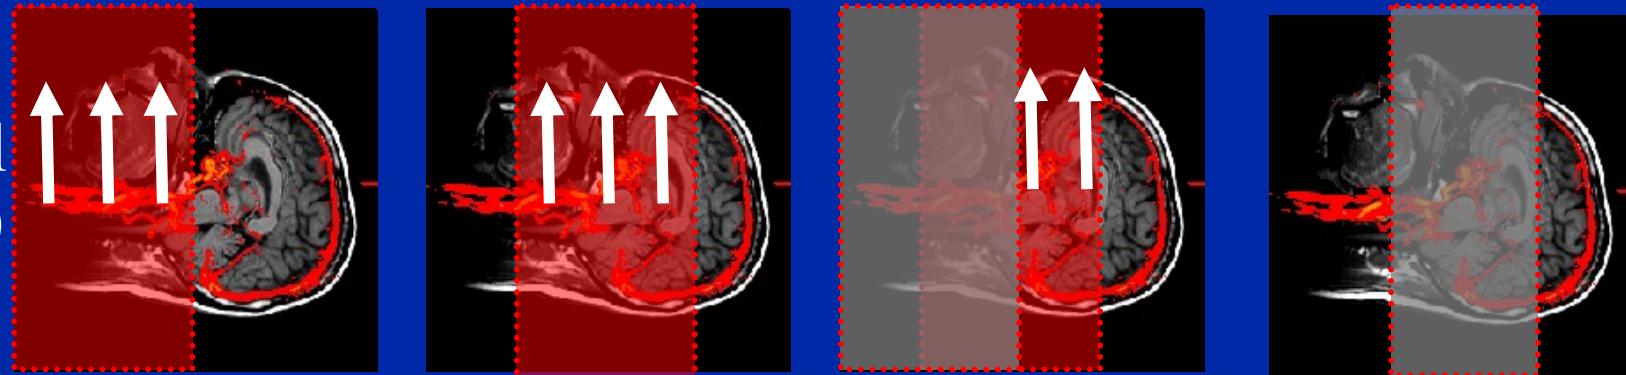


Voxel Label



View Control



ASL: Pulsed Labeling (Q2TIPS)

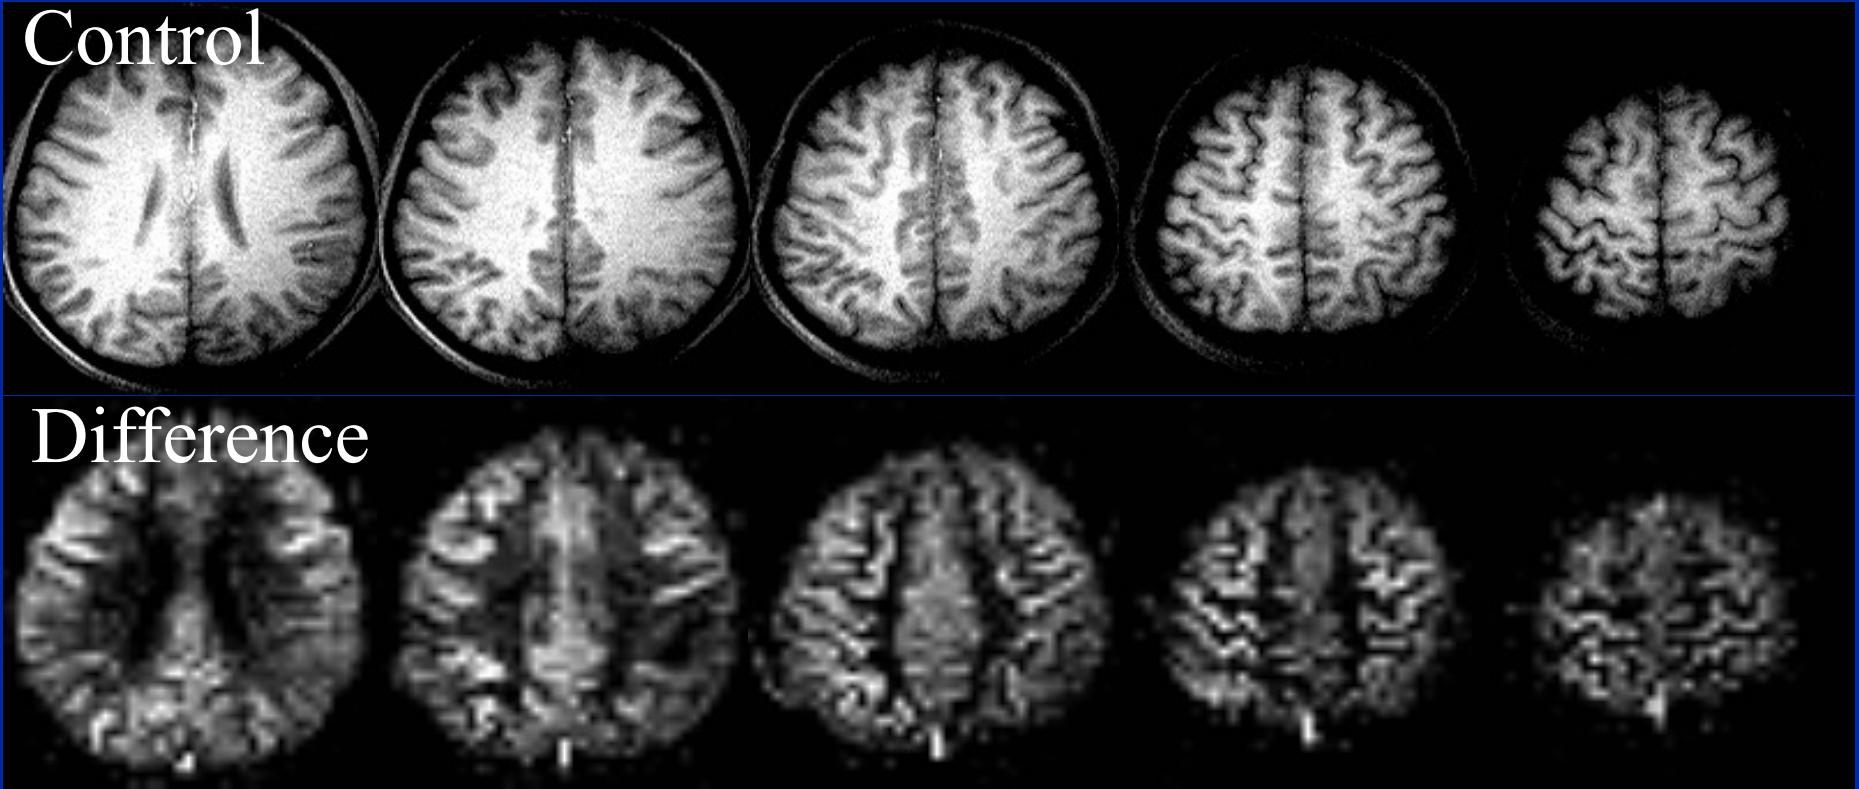

Advantages:

High tagging efficiency


Low SAR

Ease of implementation


Disadvantage:

Limited coverage

ASL: Continuous Labeling (Flow-driven Adiabatic Fast Passage)

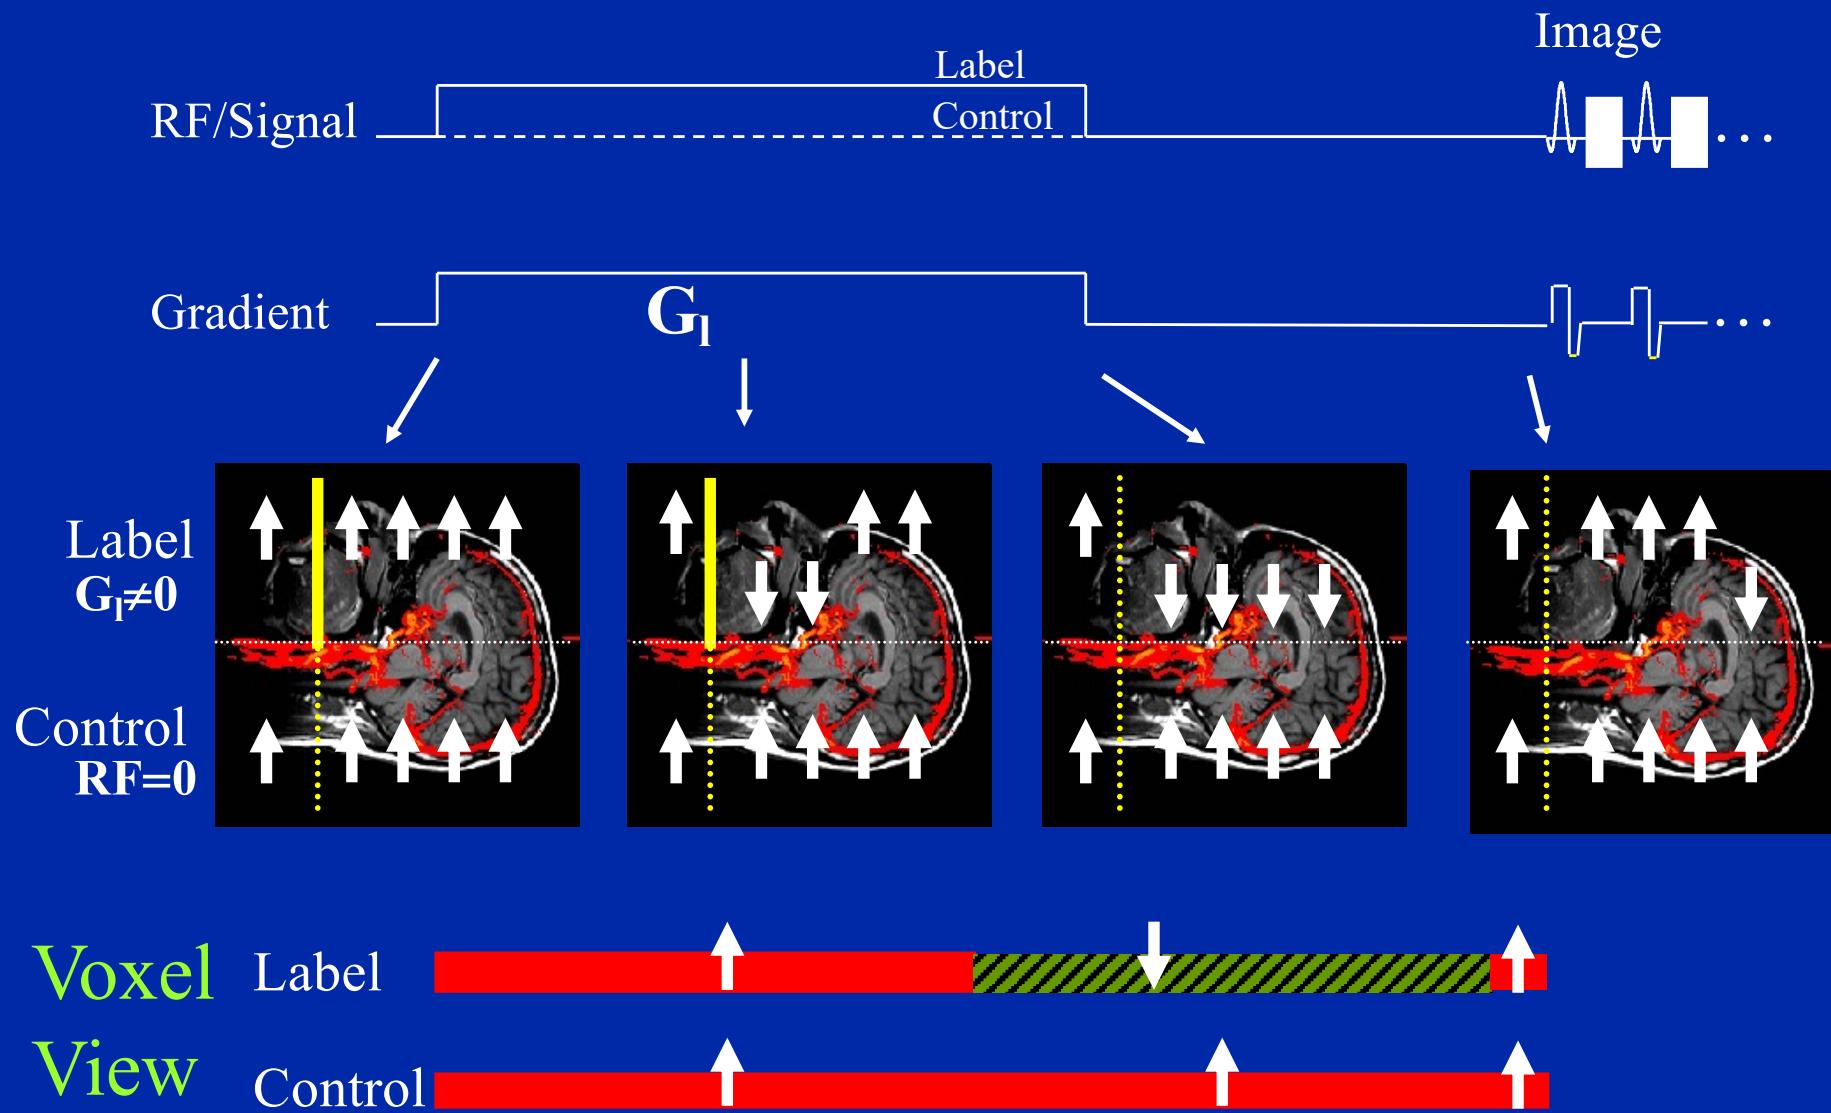

Continuous ASL: Neck Labeling Coil

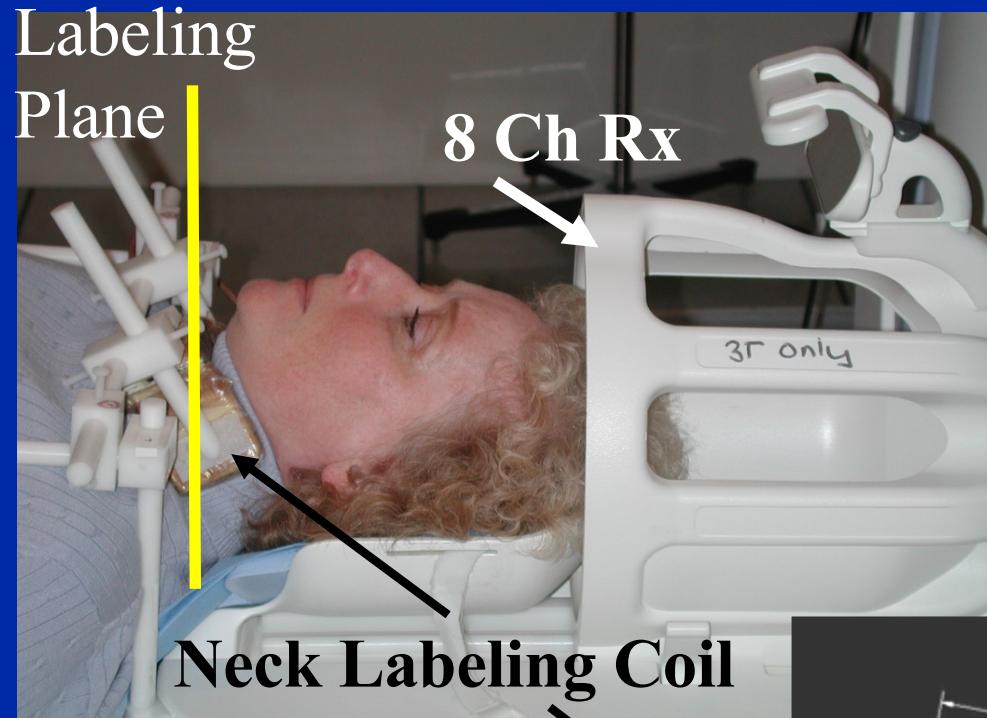


Advantages:




- Whole brain coverage
- High labeling efficiency
- Lower SAR

Disadvantage:

- Requires special hardware

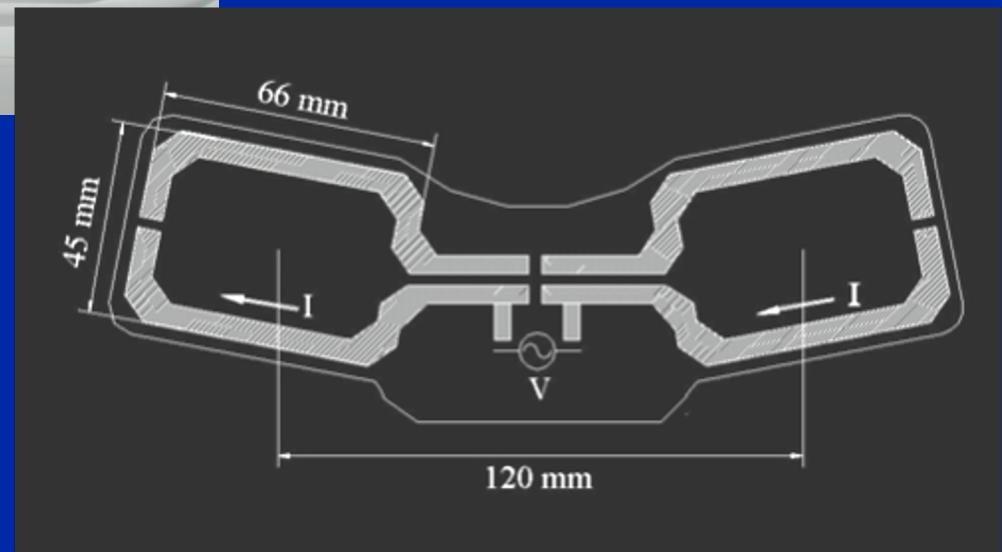

CASL with a Neck Labeling Coil: Multi-shot 3D-FSE Spiral

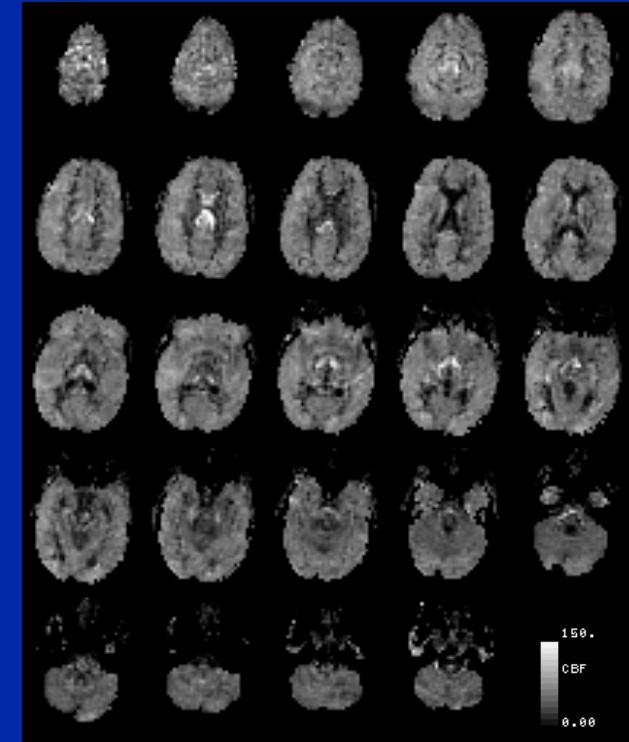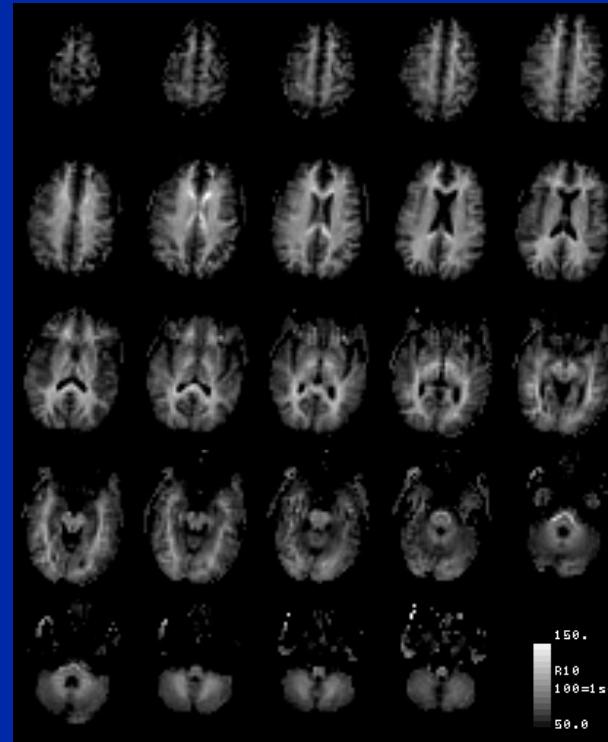
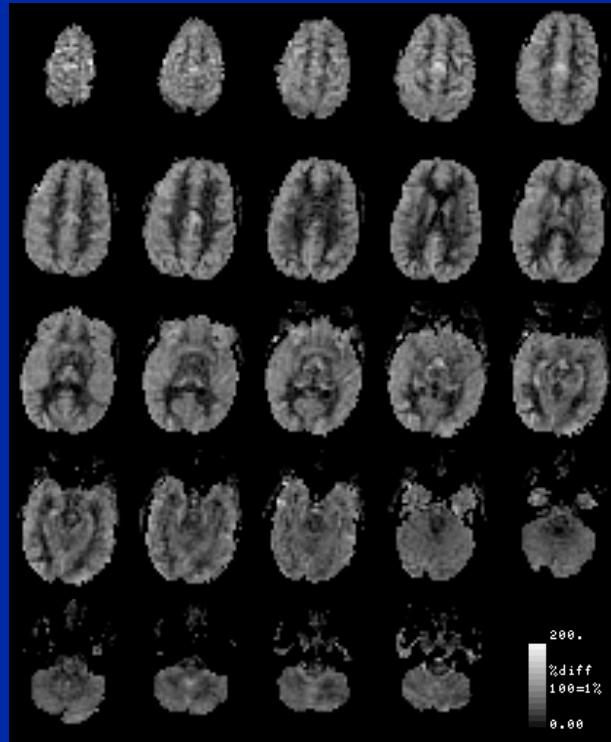


3T, Head Coil, 3D-FSE, $3.7 \times 3.7 \times 5 \text{ mm}^3$

8 shots, TR 5.9 s, Label dur 4.1 s, PL delay 1.64 s, Backgr supp
6 min 22 sec


Talagala et al, *MRM* 52: 131-140 (2004)

Continuous ASL: Neck Labeling Coil

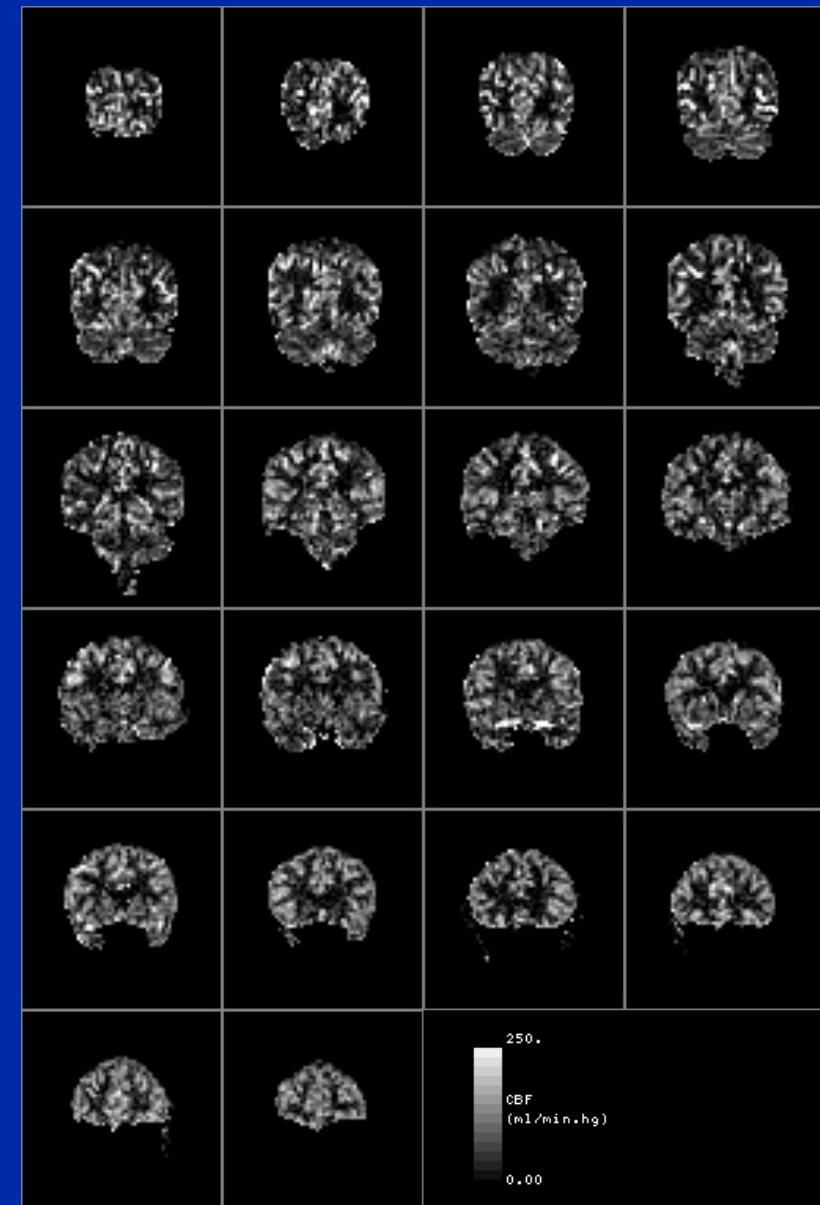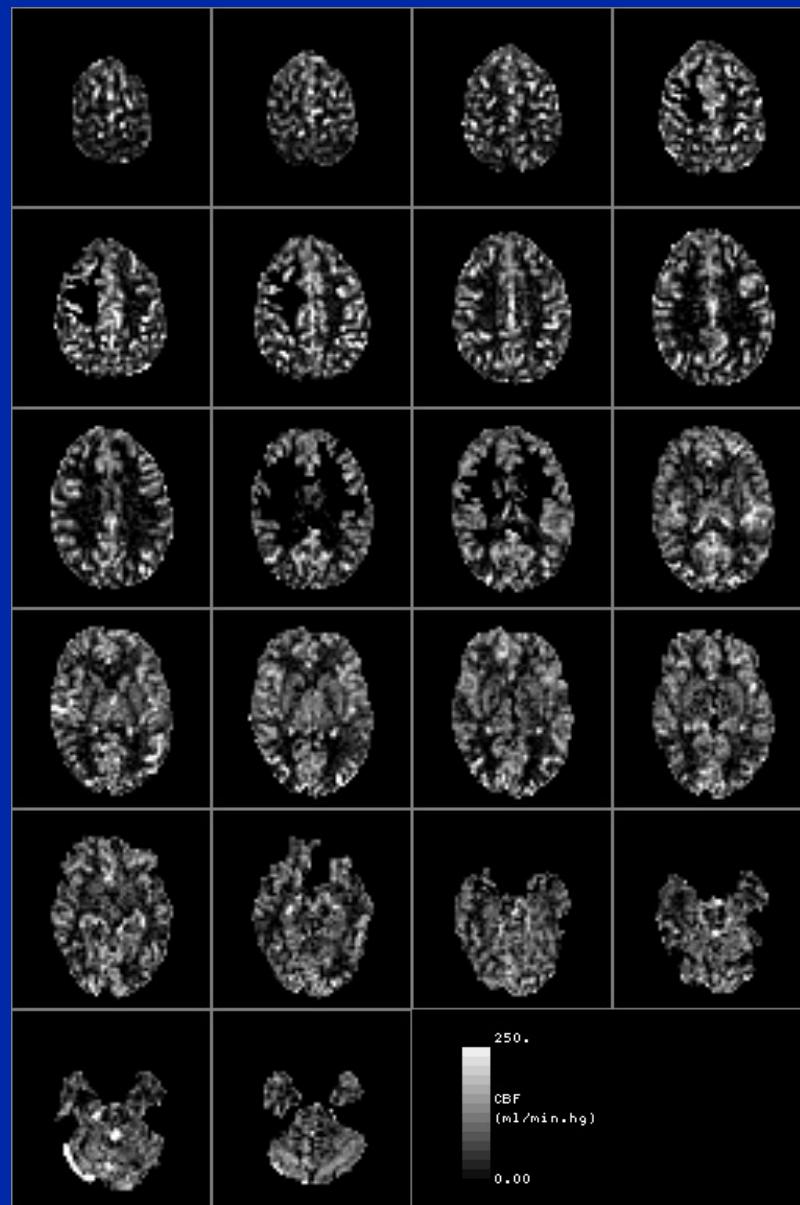

3T, 8 Ch Rx, 2D EPI, 3 x 3 x 3 mm³, TE/TR 13 ms/5 s, 4.5 minutes


CASL with a Neck Labeling Coil: Hemangioblastomas

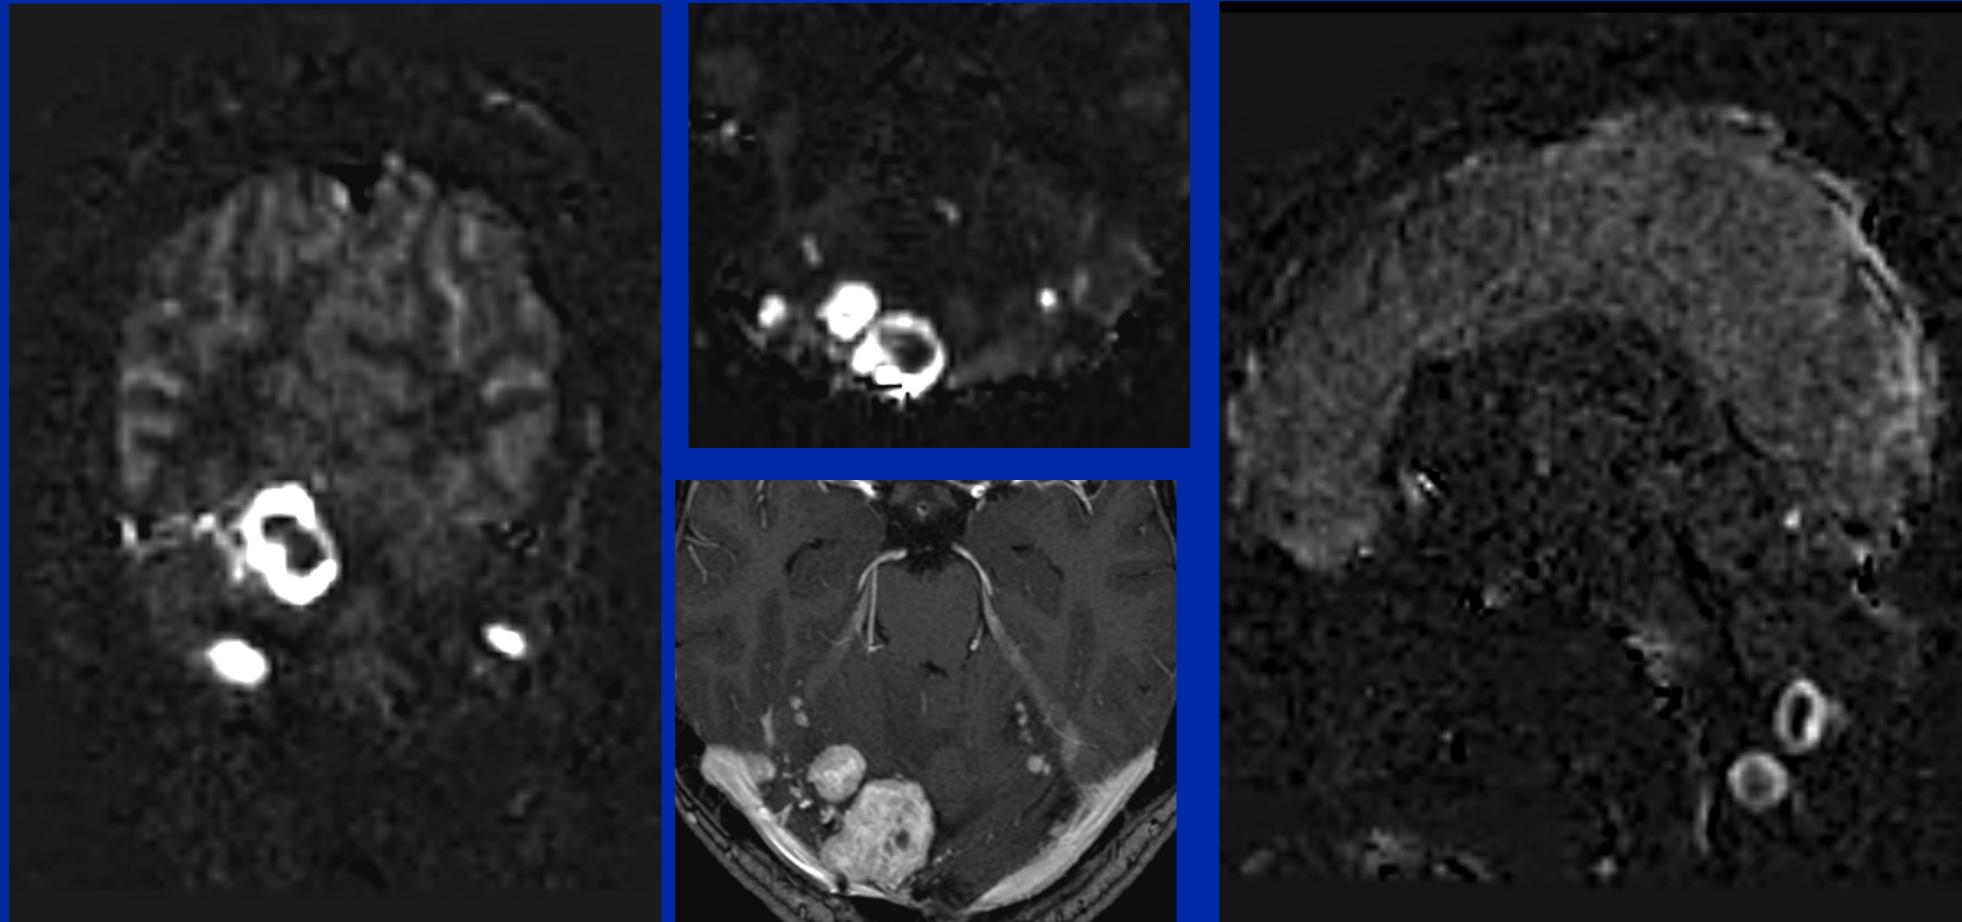

3T, 8 Ch Rx, 2D EPI, 1.5 x 1.5 x 3 mm³
TE/TR 16 ms/5 s, LD/PLD 3 s/1.6 s
10 minutes

CASL Perfusion MRI at 7 T

Volume
Tx Coil

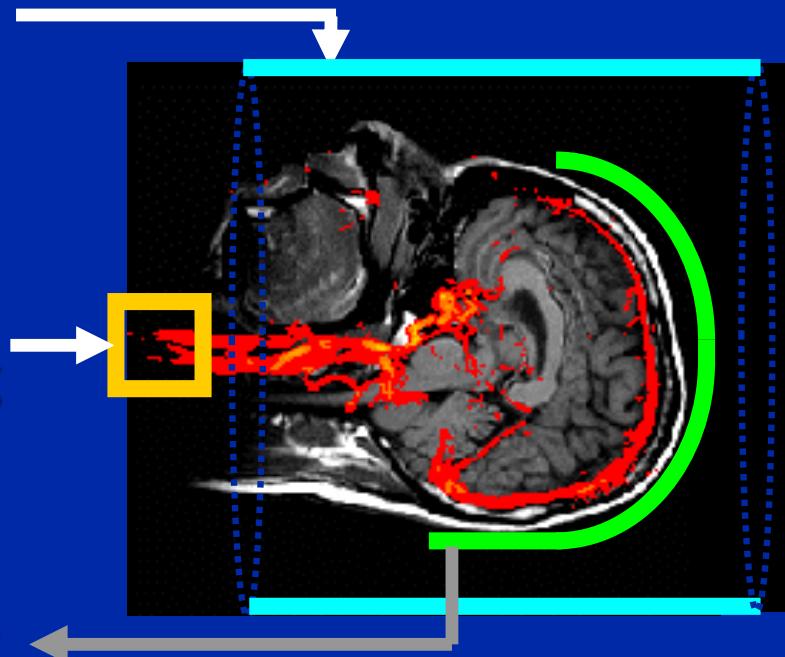


Surface
Labeling
Coil

Head Rx
Array
Coil




Tx Volume / 8 Ch Rx Array

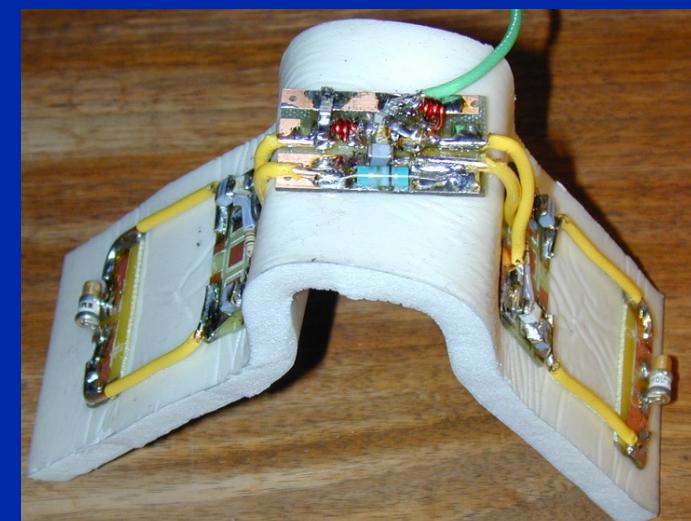


Neck Labeling Coil

7T CASL with a Neck Labeling Coil

Control (RF off) - Label (RF +ve offset)

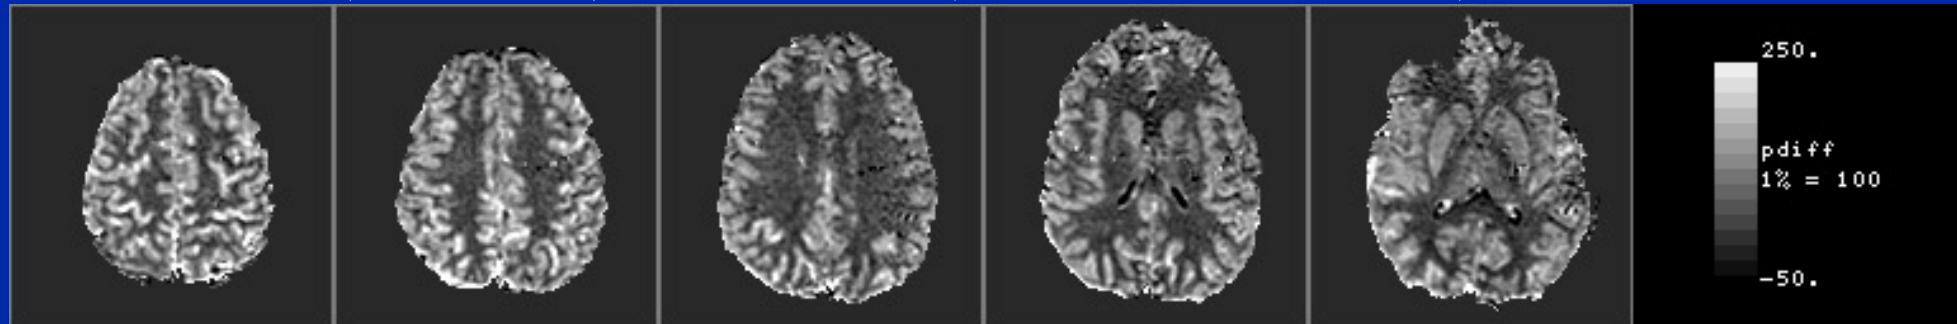


Control (RF off) - Label (RF -ve offset)

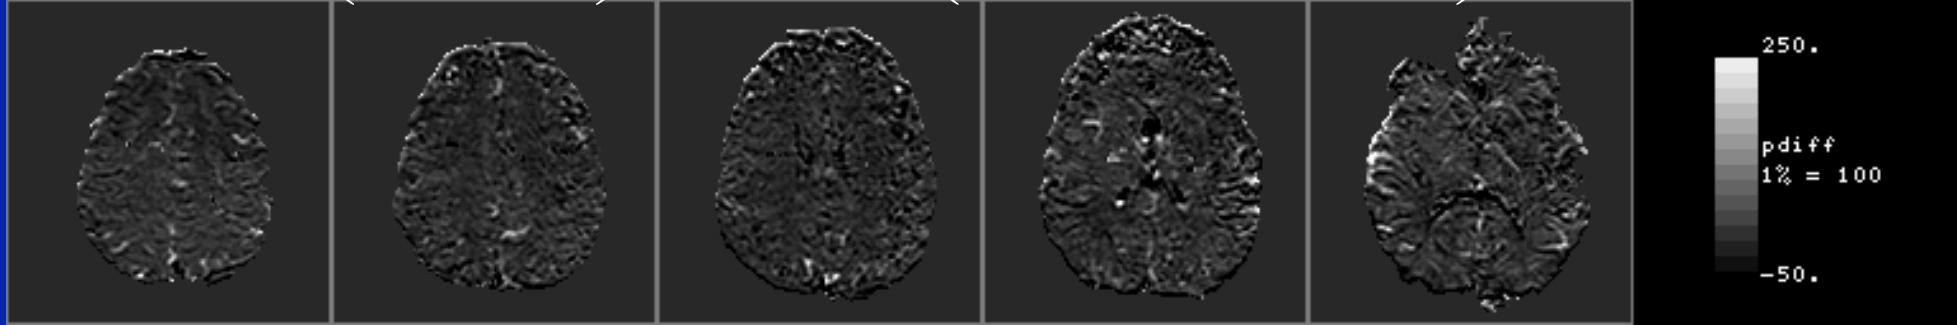

7T, 8 Ch Rx, 2D EPI, 2 x 2 x 3 mm³
TE/TR 13 ms/5 s, ASSET X2, LD = 3 s, PLD 1.5 s
8 minutes

Talagala et al ISMRM 2008


CASL Perfusion MRI at 7 T

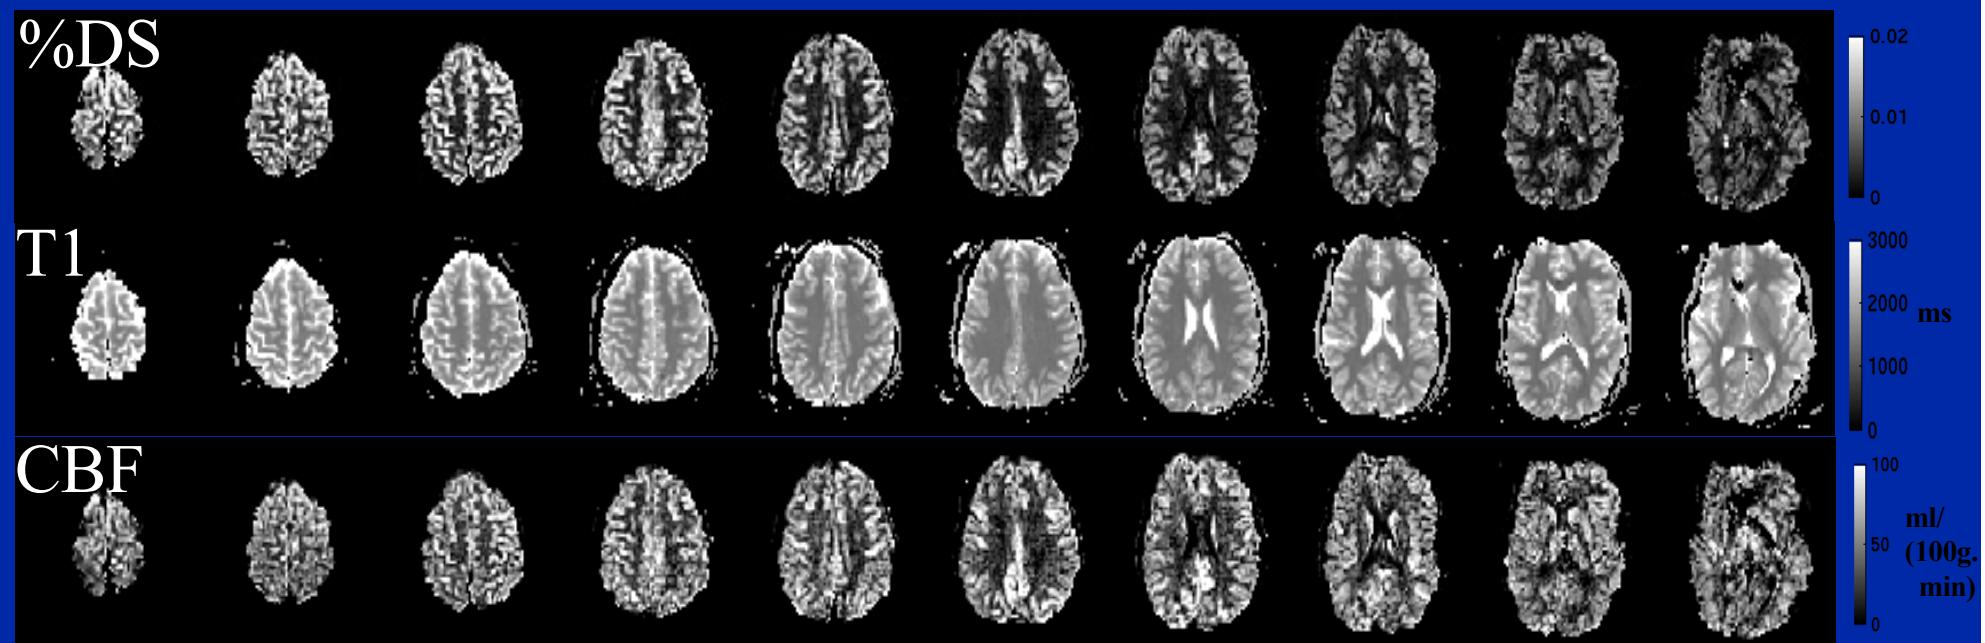

	Gray Matter	White Matter
Mean T1 (ms)	1940	1363
$\Delta S/S (\%)$	1.43 +/- 0.25	0.3 +/- 0.04
CBF (ml/min.100g)	76 +/- 11	27 +/- 2.4

7T, 8Ch Rx, 2.1 x 2.1 x 3 mm³, 9 minutes, n=5

ASL: Pseudo Continuous labeling

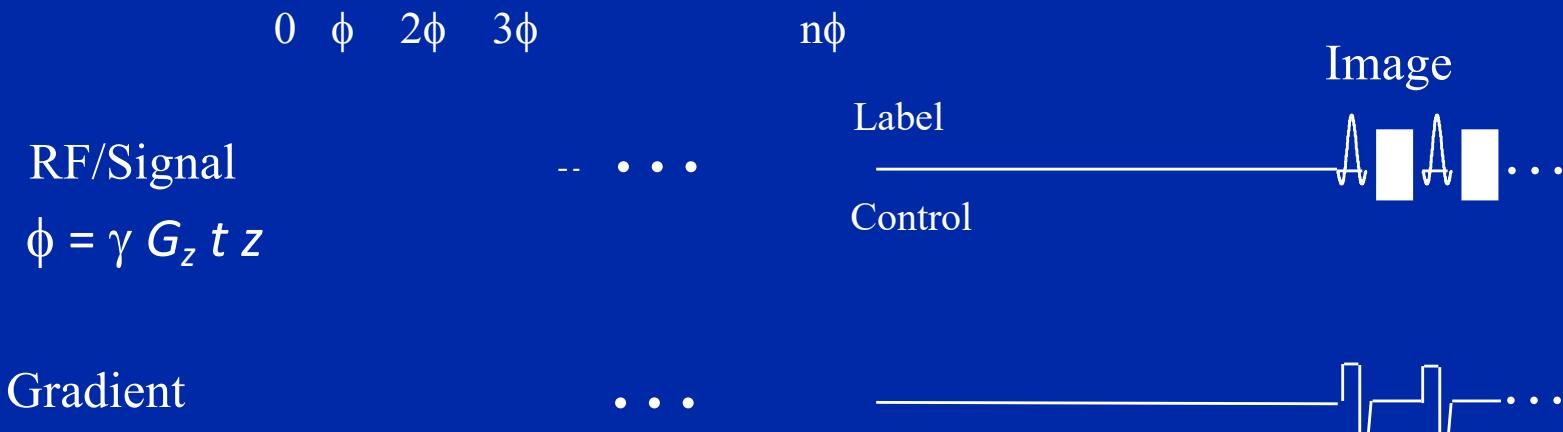


Advantages:


- Whole brain coverage
- High labeling efficiency
- Use standard hardware

Disadvantages:

- Higher SAR
- Labeling sensitive to off-resonance effects

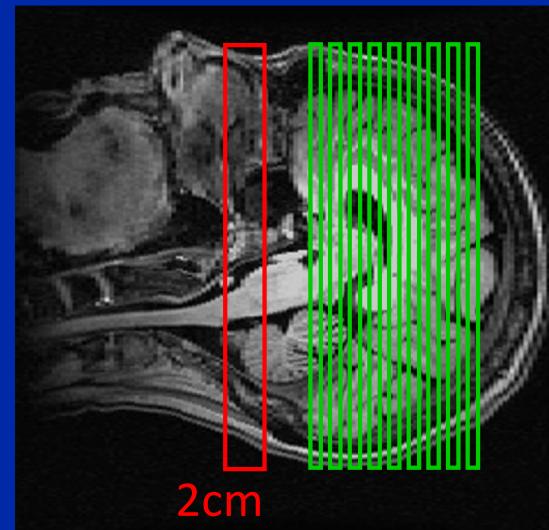


Pseudo Continuous ASL: 3T data

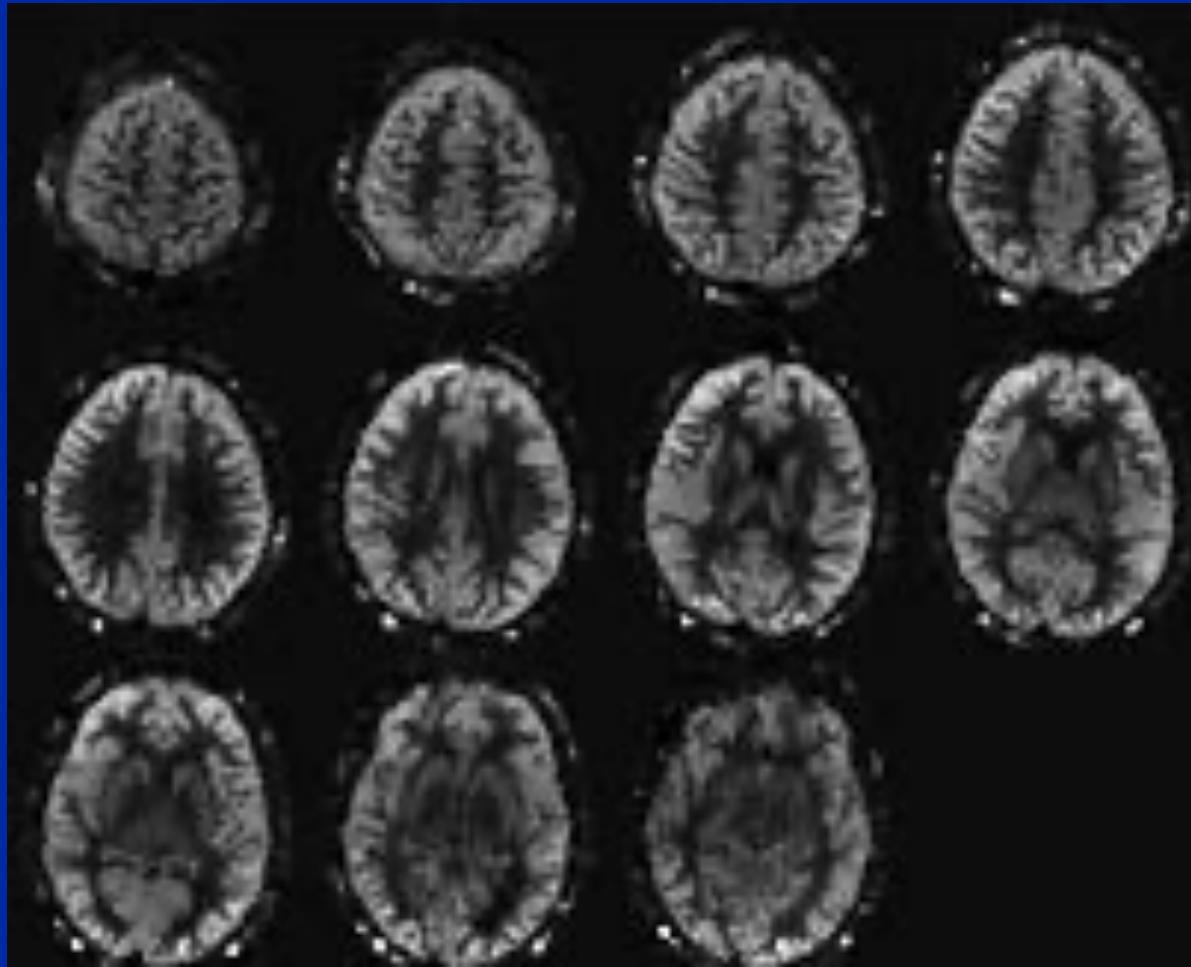

3T
3.6 x 3.6 x 5 mm³
Gradient-echo EPI
TE/TR = 20.8/5000 ms
 $\tau/w = 2500/1700$ ms
Scan time 5:00



Pseudo Continuous ASL: 7T data

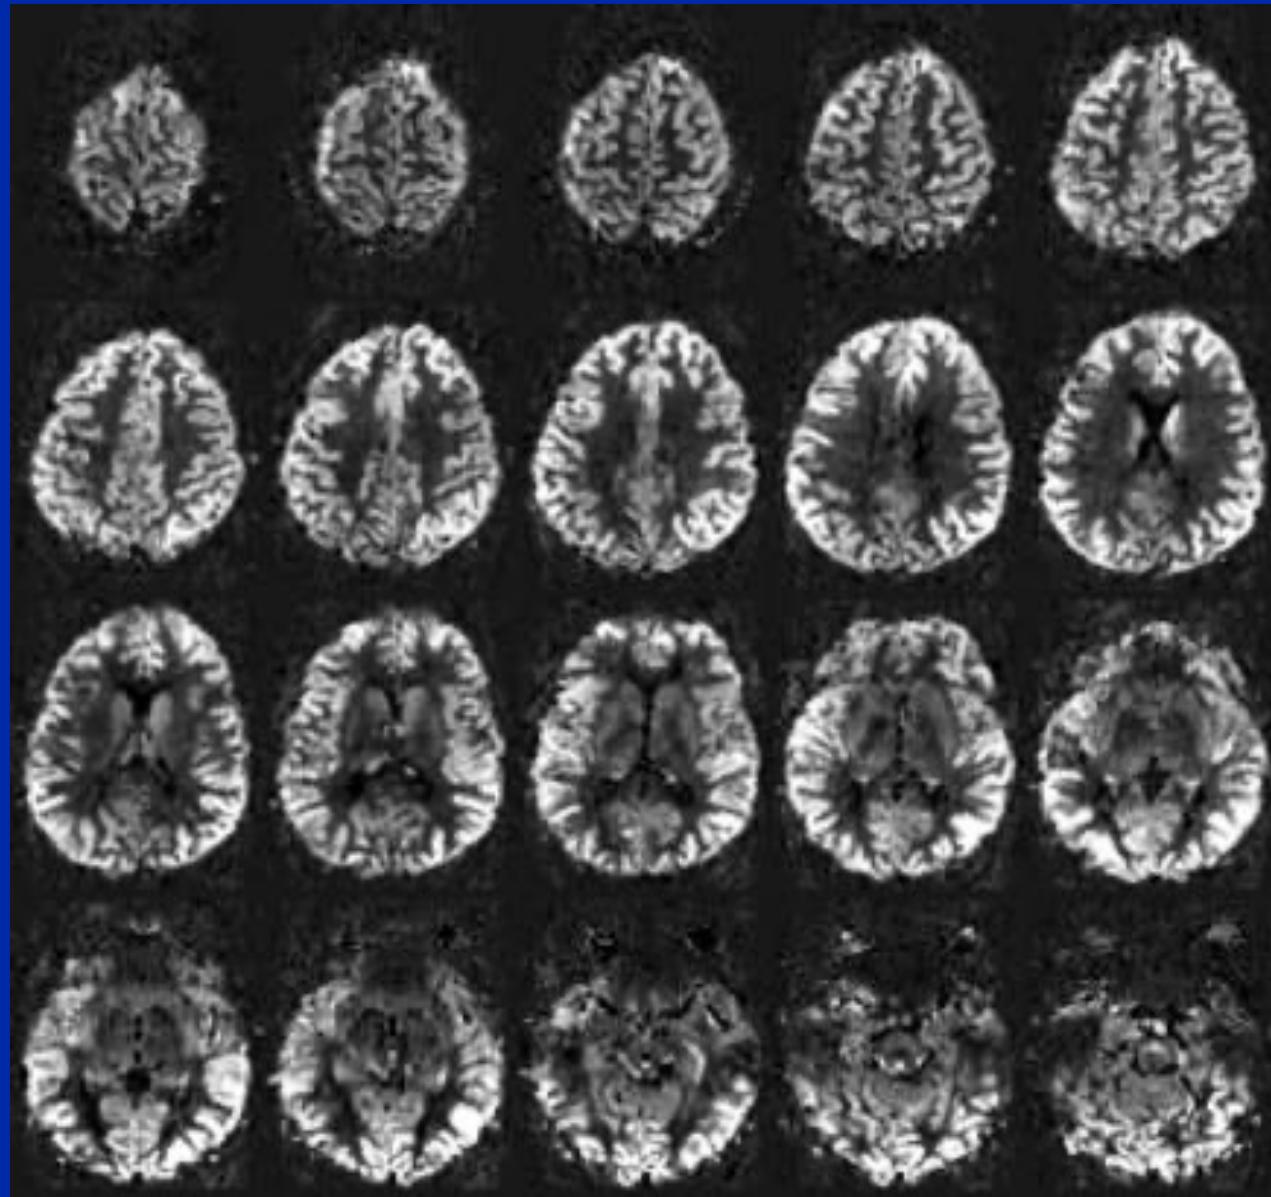

7T
2.3 x 2.3 x 3 mm³
Gradient-echo EPI
TE/TR = 20.8/5100 ms
t/w = 3000/1200 ms
SENSE 3x
Scan time 4:15


Luh et al, MRM 69:402 (2013)

CASL fMRI with a Neck Labeling Coil

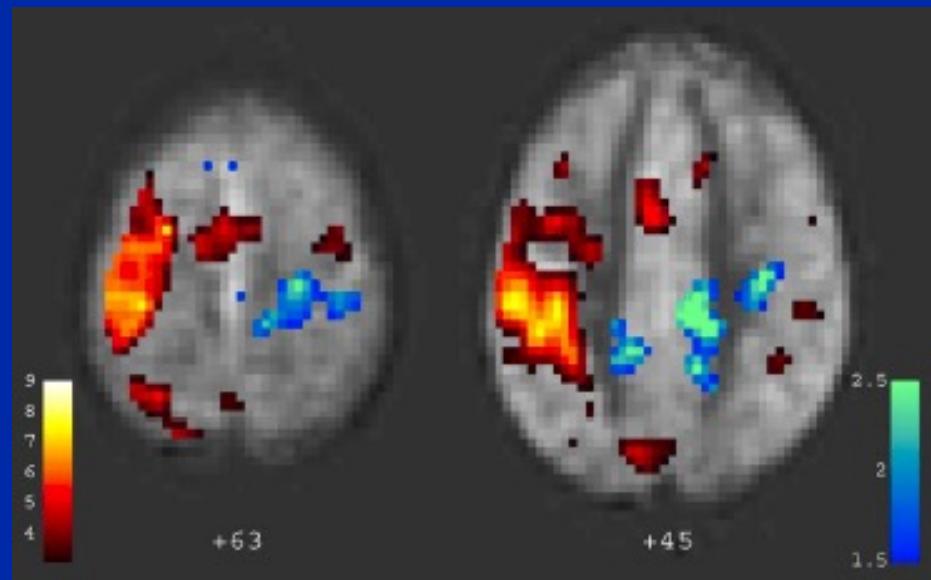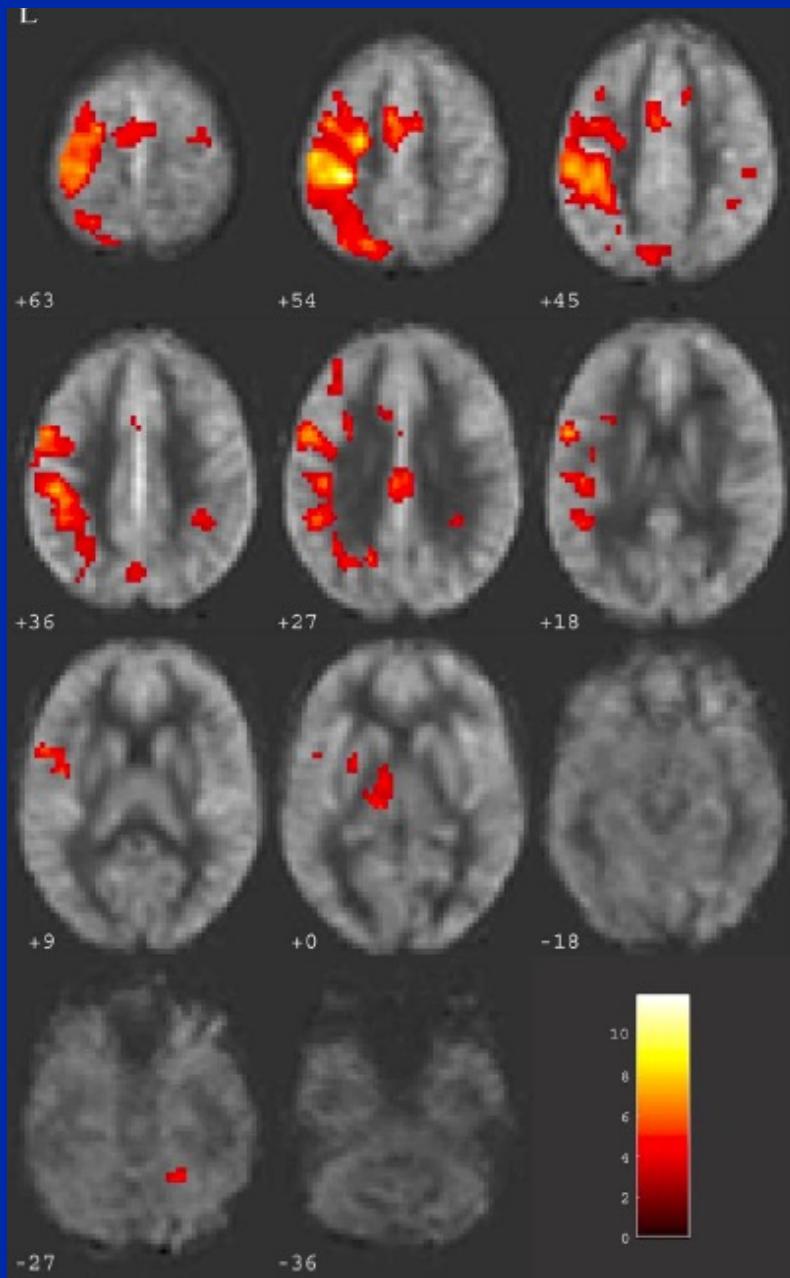


3T, Head Coil
Finger movement (0.5 Hz),
 $\{48\text{ s Task} / 48\text{ Rest}\} \times 6$, 10 min
GE EPI, $3.75 \times 3.75 \times 5\text{ mm}^3$
12 s per Cont/Label pair
SPM, Spatial normalization
smoothing (8 mm), N= 15

3T CASL Perfusion fMRI with 16 Rx

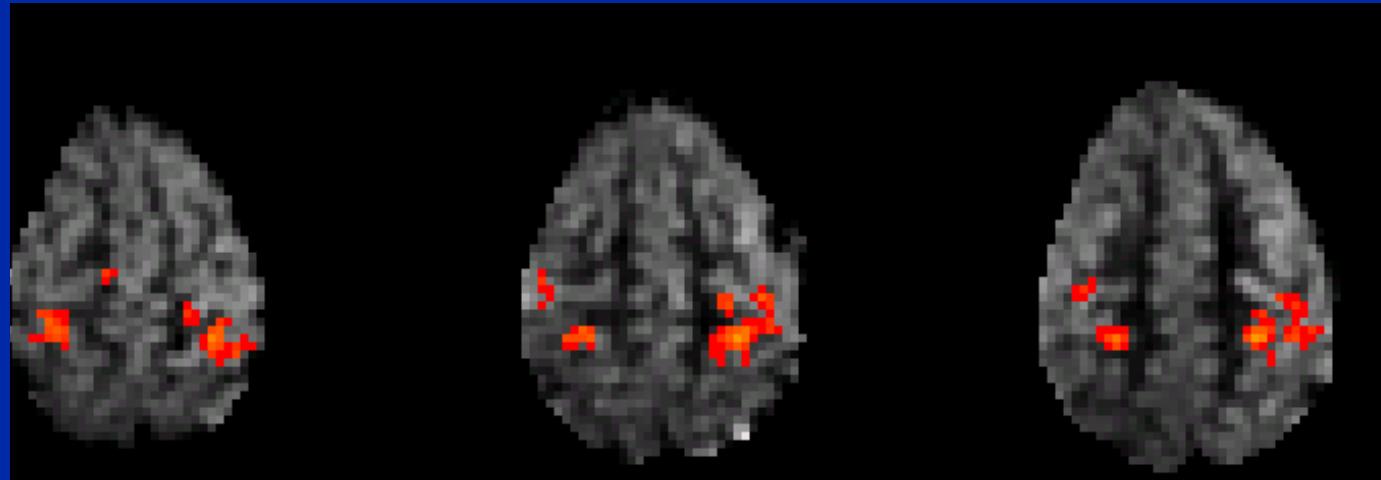

CBF
 75 ± 11
ml/(min.100g)

Δ CBF
 $78 \pm 7\%$

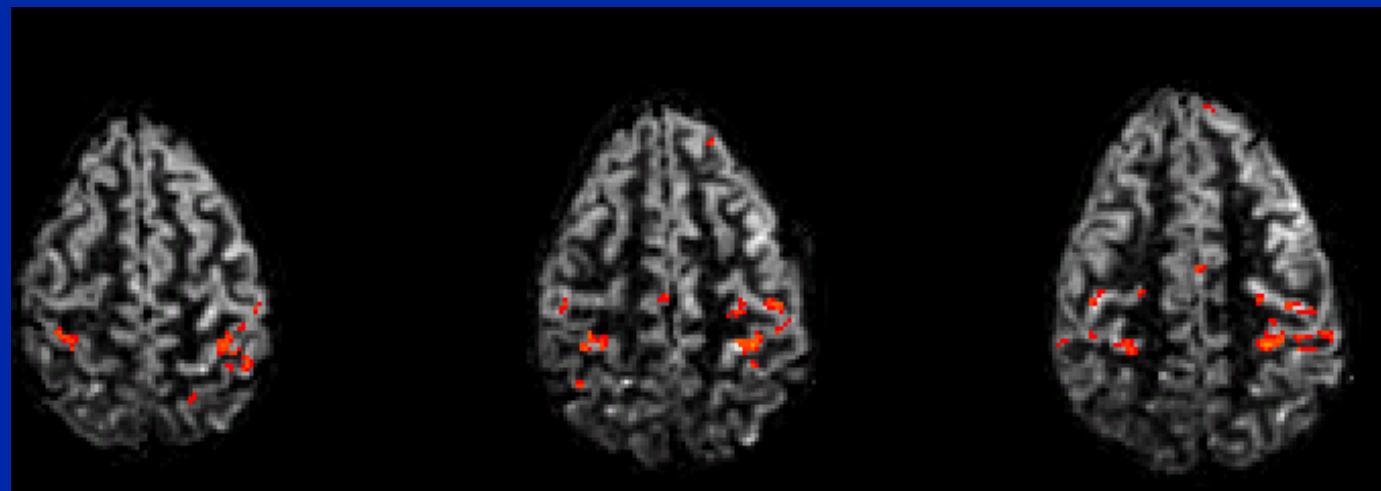


CBF
 92 ± 16
ml/(min.100g)

Δ CBF
 $102 \pm 10\%$

Finger movement (2 Hz), {40 s Rest / 40 Task} X 8, N = 6
GE EPI, TE 26 ms, 10 s per Control/Label pair, 10 min 40 sec

Functional Connectivity with ASL Perfusion

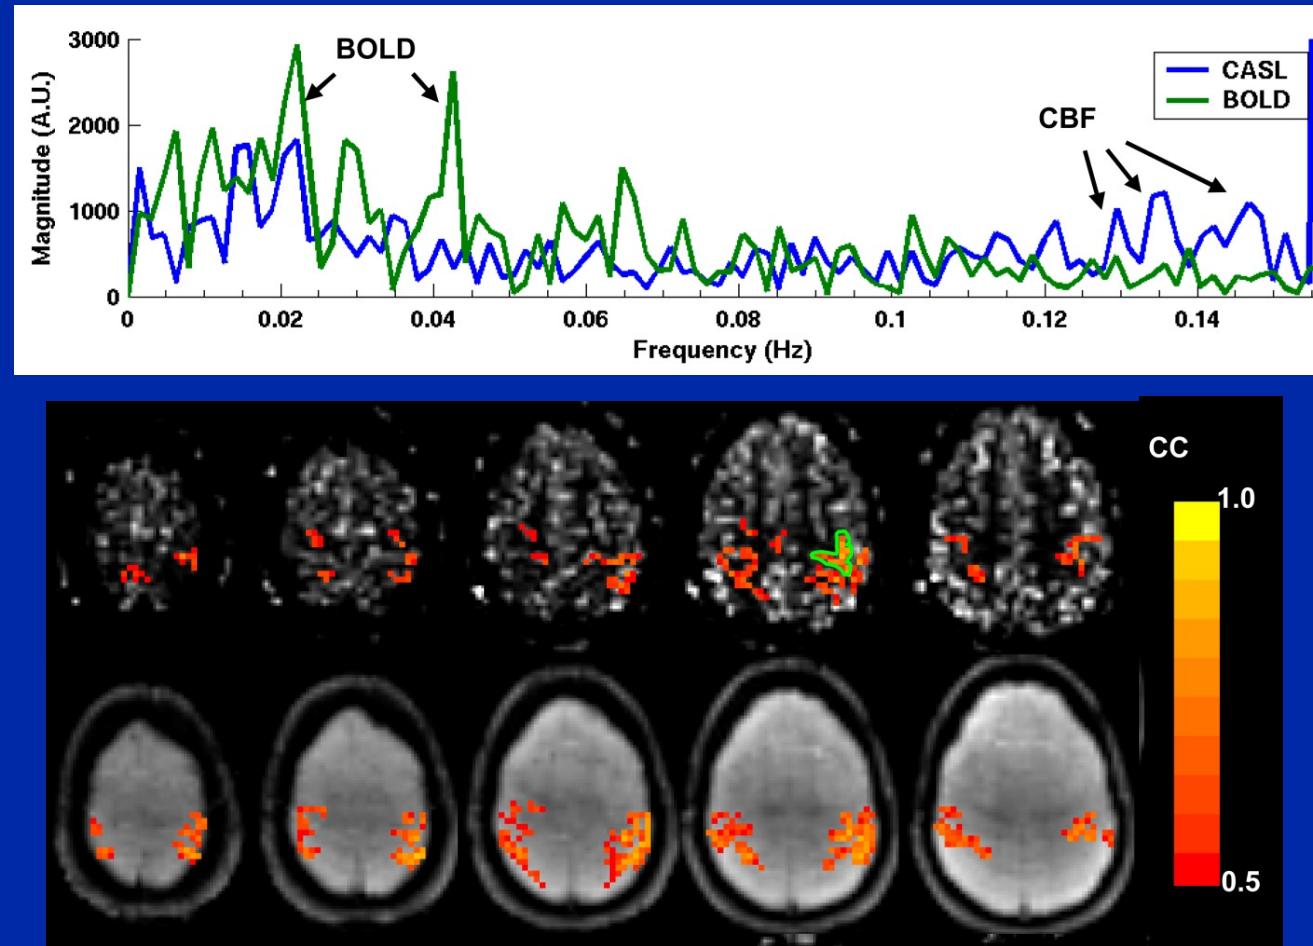


$$\Delta\text{CBF} = 29 \pm 19\% \quad \Delta\text{BOLD} = 0.26 \pm 0.14\% \quad (\text{N}=13)$$

3T, GE EPI, 16 Ch Rx, $3.75 \times 3.75 \times 3 \text{ mm}^3$

TE/TR 12.5/3200 ms, 10 min 40 sec

Functional Connectivity: BOLD, Perfusion, CMRO₂

b) Resting State:

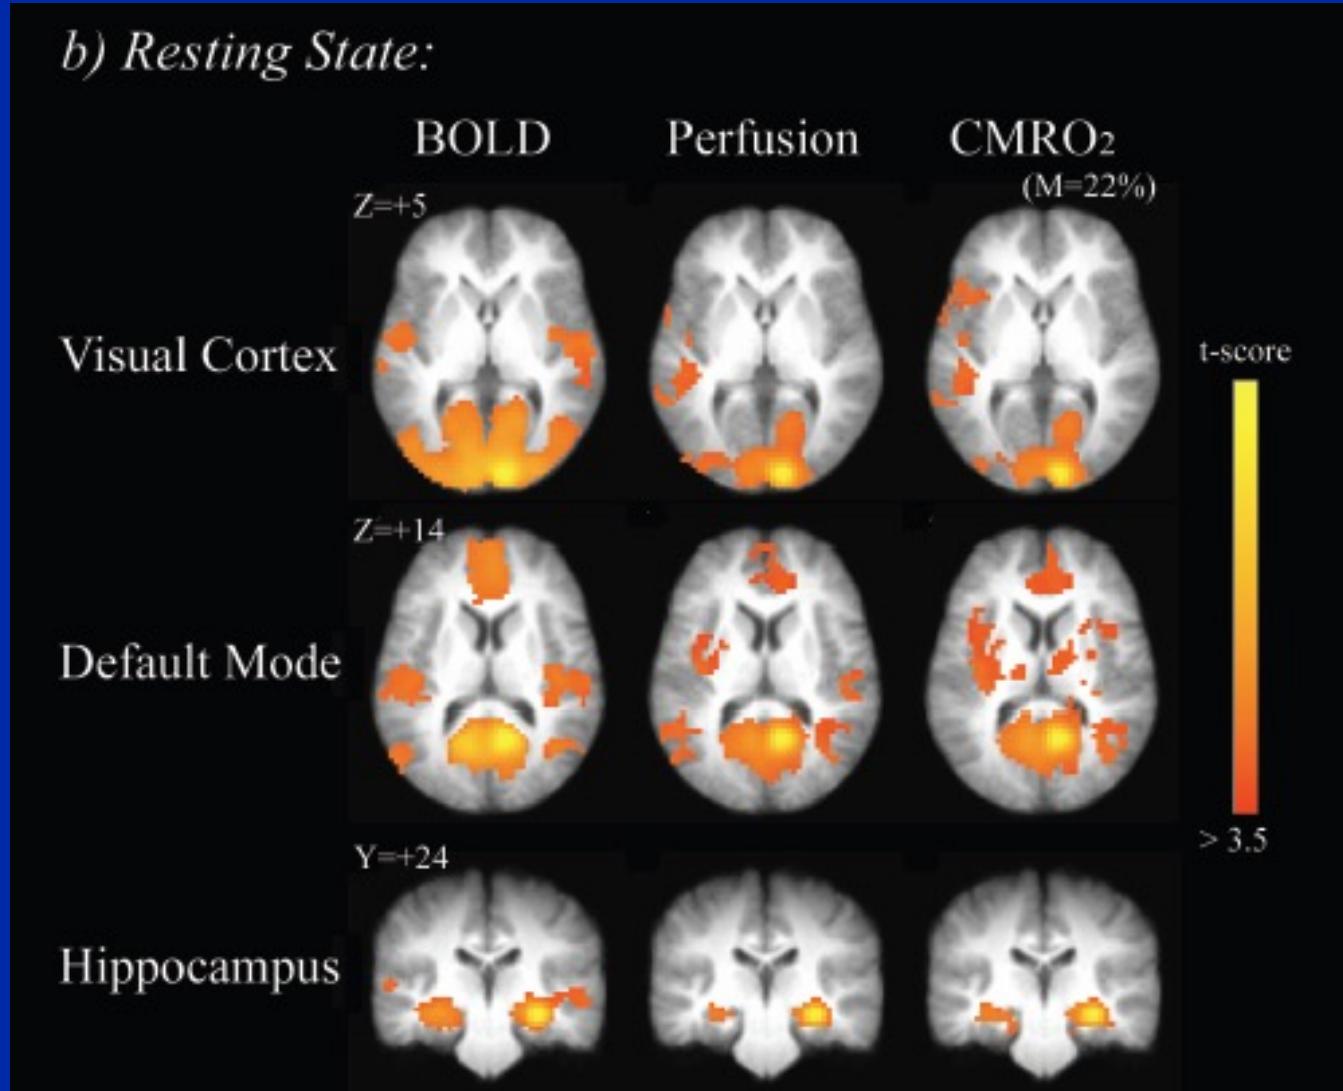

Wu et al., *NeuroImage* 45, 694 (2009)

Perfusion MRI: Summary

- ◆ Dynamic Susceptibility Contrast (DSC)
 - Requires contrast administration
 - Fast acquisition (< 2 min), whole brain coverage
 - Readily performed in clinical scanners
 - Online/Offline processing software available
 - Absolute quantification is difficult
- ◆ Arterial Spin Labeling (ASL)
 - No contrast required
 - 4-5 min acquisition, whole brain coverage
 - Absolute quantification is possible
 - Robust sequences becoming available
 - Useful for clinical and research work